

Method 508 GC/MS Date Extracted 10/9/01

Page 21

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH = 7	Count
	Lab 6th	SW.	—	✓		—	2M			
	Ret chlorane									
	MDL chlor.									
	PEL 1242									
	Spike pest				1ml					
	Spike dup pest									
	Spike TDX									
	Spike dup TDX									
	24135									20
	24214									1
Remarks										
Reviewed by, <u>JB 1/20/02</u>										
drip rate must be between 5-15 ml/min for liq-liq extractors			drip rate -							
Extraction type - <u>Sep hum</u>			Solv. lot#		NaCl lot# <u>T/2617</u>		Na2SO4 lot# <u>8024 1132604</u>			
STANDARD	INT STD LOG#									
CALIBRATION										
REF/SPIKE	<u>Chlor. 1750 PEL 1242 1503</u>									
MDL/MDRF										
Q. CHECK										
INT. STD.										
SURROGATE	<u>2064C</u>									
LPC										
ENDRIN/DDT										

Analyst Mg/AP
revision 4/12/01

Verified by _____

Reviewed by DW
Date 11/2/01

Sequence Name: C:\HPCHEM\1\SEQUENCE\OCT3001.S
 Comment: INST 209; 30Mx0.25umX0.50
 Operator: 209 GALOS
 Data Path: C:\HPCHEM\1\data\oct3001\
 Pre-Seq Cmd:
 Post-Seq Cmd:

Method Sections To Run On A Barcode Mismatch
 (X) Full Method (X) Inject Anyway
 () Reprocessing Only () Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	NP101901	
2	Sample	1	DFTPP1	NP101901	
3	Sample	1	DFTPP2	NP101901	
4	Sample	1	DFTPP3	NP101901	
5	Sample	2	CAL5A	NP101901	mix
6	Sample	3	CAL10A	NP101901	mix
7	Sample	4	CAL25	NP101901	mix
8	Sample	5	CAL40	NP101901	mix
9	Sample	6	CAL80	NP101901	mix
10	Sample	7	CAL100	NP101901	mix
11	Sample	8	LB	NP101901	lab blk 10/1
12	Sample	9	23798	NP101901	gc/ms unknown
13	Sample	10	23799	NP101901	gc/ms unknown
14	Sample	11	23837	NP101901	gc/ms unknown
15	Sample	12	23838	NP101901	gc/ms unknown
16	Sample	13	23839	NP101901	gc/ms unknown
17	Sample	14	23842	NP101901	gc/ms unknown
18	Sample	15	23843	NP101901	gc/ms unknown
19	Sample	16	23836	NP101901	gc/ms unknown
20	Sample	17	23797	NP101901	gc/ms unknown
21	Sample	18	23833	NP101901	gc/ms unknown
22	Sample	19	23834	NP101901	gc/ms unknown
23	Sample	20	23835	NP101901	gc/ms unknown
24	Sample	1	DFTPP4	NP101901	
25	Sample	21	LBA	NP101901	lab blk 10/9
26	Sample	22	24135	NP101901	gc/ms unknown
27	Sample	23	24214	NP101901	gc/ms unknown

DFTPP

Data File : C:\HPCHEM\1\DATA\OCT3001\DFTPP4.D

Acq On : 31 Oct 2001 10:28 am

Sample :

Misc :

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

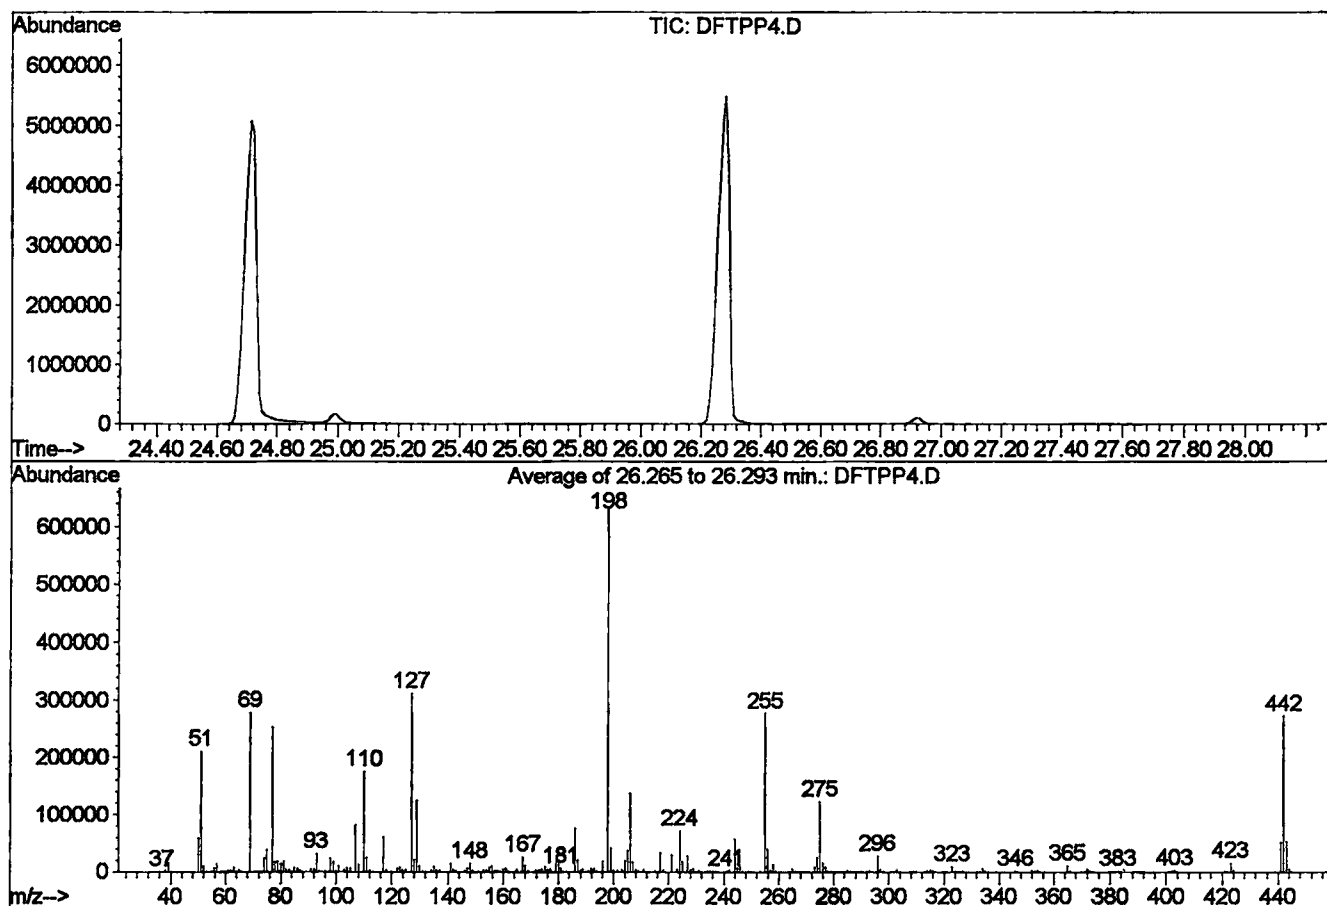

Spectrum Information: Average of 26.265 to 26.293 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	33.3	211152	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	44.0	278976	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	49.2	312256	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	634672	PASS
199	198	5	9	6.6	41866	PASS
275	198	10	30	19.3	122736	PASS
365	198	1	100	1.6	10137	PASS
441	443	0.01	100	97.3	51302	PASS
442	198	40	110	43.1	273232	PASS
443	442	17	23	19.3	52724	PASS

DFTPP4.D NP103001.M

Thu Nov 01 10:26:58 2001