

User: Galos, Marie
 Westchester Dept. of Labs & Research
 Date: 11/06/2001 Time: 12:16:20

Sample: AD24218
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 11/6/01 12:15 Ended: 11/6/01 12:15 Analyst: MG
 Page: 1

	Component Name	Via	Result
1	Other unknown compounds		see comment

Comments for Sample AD24218 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Galos, Marie

Date: 11-06-2001 Time: 12:16:27

A scan of the extract prepared for the 508 analysis, from 35-550 amu using a mass spectrometer, does not reveal the presence of non-target compounds.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV0101\24218.D
 Acq On : 1 Nov 2001 6:55 pm
 Sample : gc/ms unknown
 Misc :
 MS Integration Params: RTEINT.P
 Quant Time: Nov 6 11:34 2001

Vial: 5
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: NP101901.RES

Quant Method : C:\HPCHEM\1\METHODS\NP101901.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Tue Oct 23 10:12:13 2001
 Response via : Initial Calibration
 DataAcq Meth : NP101901

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	11.72	152	562930	20.00	ug/l	0.00
19) Naphthalene-d8	15.32	136	2235943	20.00	ug/l	-0.02
31) Acenaphthene-d10	20.59	164	1072026	20.00	ug/l	-0.02
49) Phenanthrene-d10	25.02	188	1586177	20.00	ug/l	-0.02
59) Chrysene-d12	33.06	240	1019194	20.00	ug/l	0.00
68) Perylene-d12	37.15	264	690334	20.00	ug/l	0.00

System Monitoring Compounds

4) 2-Fluorophenol	0.00	112	0	0.00	ug/l	
Spiked Amount	75.000		Recovery	=	0.00%	
5) Phenol-d5	0.00	99	0	0.00	ug/l	
Spiked Amount	75.000		Recovery	=	0.00%	
6) 2-Chlorophenol-d4	11.72	132	270	0.01	ug/l	0.48
Spiked Amount	75.000		Recovery	=	0.01%	
7) 1,2-Dichlorobenzene-d4	12.23	152	5878	0.28	ug/l	-0.02
Spiked Amount	50.000		Recovery	=	0.56%	
20) Nitrobenzene-d5	0.00	82	0	0.00	ug/l	
Spiked Amount	50.000		Recovery	=	0.00%	
32) 2-Fluorobiphenyl	18.75	172	2249	0.04	ug/l	0.13
Spiked Amount	50.000		Recovery	=	0.08%	
33) 2,4,6-Tribromophenol	0.00	330	0	0.00	ug/l	
Spiked Amount	75.000		Recovery	=	0.00%	
62) Terphenyl-d14	0.00	244	0	0.00	ug/l	
Spiked Amount	50.000		Recovery	=	0.00%	

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Pyridine	0.00	79	0	N.D.		
3) N-nitroso-dimethyl amine	0.00	74	0	N.D.		
8) Phenol	0.00	94	0	N.D.		
9) bis(2-Chloroethyl) ether	0.00	93	0	N.D.		
10) 2-Chlorophenol	0.00	128	0	N.D.		
11) 1,3-Dichlorobenzene	0.00	146	0	N.D.		
12) 1,4-Dichlorobenzene	0.00	146	0	N.D.		
13) 1,2-Dichlorobenzene	0.00	146	0	N.D.		
14) 2-Methylphenol	0.00	108	0	N.D.		
15) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.		
16) 3&4-Methylphenol	0.00	108	0	N.D.		
17) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.		
18) Hexachloroethane	0.00	117	0	N.D.		
21) Nitrobenzene	0.00	77	0	N.D.		
22) Isophorone	0.00	82	0	N.D.		

(#) = qualifier out of range (m) = manual integration

24218.D NP103001.M Tue Nov 06 11:34:31 2001

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV0101\24218.D
 Acq On : 1 Nov 2001 6:55 pm
 Sample : gc/ms unknown
 Misc :
 MS Integration Params: RTEINT.P
 Quant Time: Nov 6 11:34 2001

Vial: 5
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: NP101901.RES

Quant Method : C:\HPCHEM\1\METHODS\NP101901.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Tue Oct 23 10:12:13 2001
 Response via : Initial Calibration
 DataAcq Meth : NP101901

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
23) 2-Nitrophenol	0.00	139	0	N.D.		
24) 2,4-Dimethylphenol	0.00	107	0	N.D.		
25) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.		
26) 2,4-Dichlorophenol	0.00	162	0	N.D.		
27) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.		
28) Naphthalene	15.38	128	326	N.D.		
29) Hexachlorobutadiene	0.00	225	0	N.D.		
30) 4-Chloro-3-methylphenol	0.00	107	0	N.D.		
34) Hexachlorocyclopentadiene	0.00	237	0	N.D.		
35) 2,4,6-Trichlorophenol	0.00	196	0	N.D.		
36) 2,4,5-Trichlorophenol	0.00	196	0	N.D.		
37) 2-Chloronaphthalene	0.00	162	0	N.D.		
38) Dimethylphthalate	20.20	163	816	N.D.		
39) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d	
40) Acenaphthylene	0.00	152	0	N.D.		
41) Acenaphthene	0.00	153	0	N.D.		
42) 2,4-Dinitrophenol	0.00	184	0	N.D.		
43) 4-Nitrophenol	0.00	65	0	N.D.		
44) 2,4-Dinitrotoluene	0.00	165	0	N.D.		
45) Diethylphthalate	22.11	149	522	N.D.		
46) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.		
47) Fluorene	0.00	166	0	N.D.		
48) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.		
50) 4,6-Dinitro-2-methylphenol	0.00	198	0	N.D.		
51) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
52) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
53) Hexachlorobenzene	0.00	284	0	N.D.		
54) Pentachlorophenol	0.00	266	0	N.D.		
55) Phenanthrene	25.02	178	405	N.D.		
56) Anthracene	25.02	178	405	N.D.		
57) Di-n-butylphthalate	27.03	149	10098	N.D.		
58) Fluoranthene	0.00	202	0	N.D.		
60) 3,3'-Dichlorobenzidine	0.00	252	0	N.D.		
61) Benzidine	0.00	184	0	N.D.		
63) Pyrene	0.00	202	0	N.D.		
64) Butylbenzylphthalate	0.00	149	0	N.D.		
65) Benzo(a)anthracene	33.05	228	2690	N.D.		
66) Bis(2-ethylhexyl)phthalate	33.34	149	2362	N.D.		
67) Chrysene	33.05	228	2690	N.D.		
69) Di-n-Octylphthalate	0.00	149	0	N.D.		
70) Benzo(b)fluoranthene	0.00	252	0	N.D.		

(#) = qualifier out of range (m) = manual integration

24218.D NP103001.M Tue Nov 06 11:34:36 2001

Page 2

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV0101\24218.D

Vial: 5

Acq On : 1 Nov 2001 6:55 pm

Operator: 209 GALOS

Sample : gc/ms unknown

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Nov 6 11:34 2001

Quant Results File: NP101901.RES

Quant Method : C:\HPCHEM\1\METHODS\NP101901.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Tue Oct 23 10:12:13 2001

Response via : Initial Calibration

DataAcq Meth : NP101901

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
71) Benzo(k)fluoranthene	0.00	252	0	N.D.		
72) Benzo(a)pyrene	37.15	252	2876	N.D.		
73) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
74) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
75) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

24218.D NP103001.M Tue Nov 06 11:34:37 2001

Page 3


Quantitation Report

Data File : C:\HPCHEM\1\DATA\NOV0101\24218.D
Acq On : 1 Nov 2001 6:55 pm
Sample : gc/ms unknown
Misc :
MS Integration Params: RTEINT.P
Quant Time: Nov 6 11:34 2001

Vial: 5
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: NP101901.RES

Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Fri Nov 02 16:41:16 2001
Response via : Initial Calibration

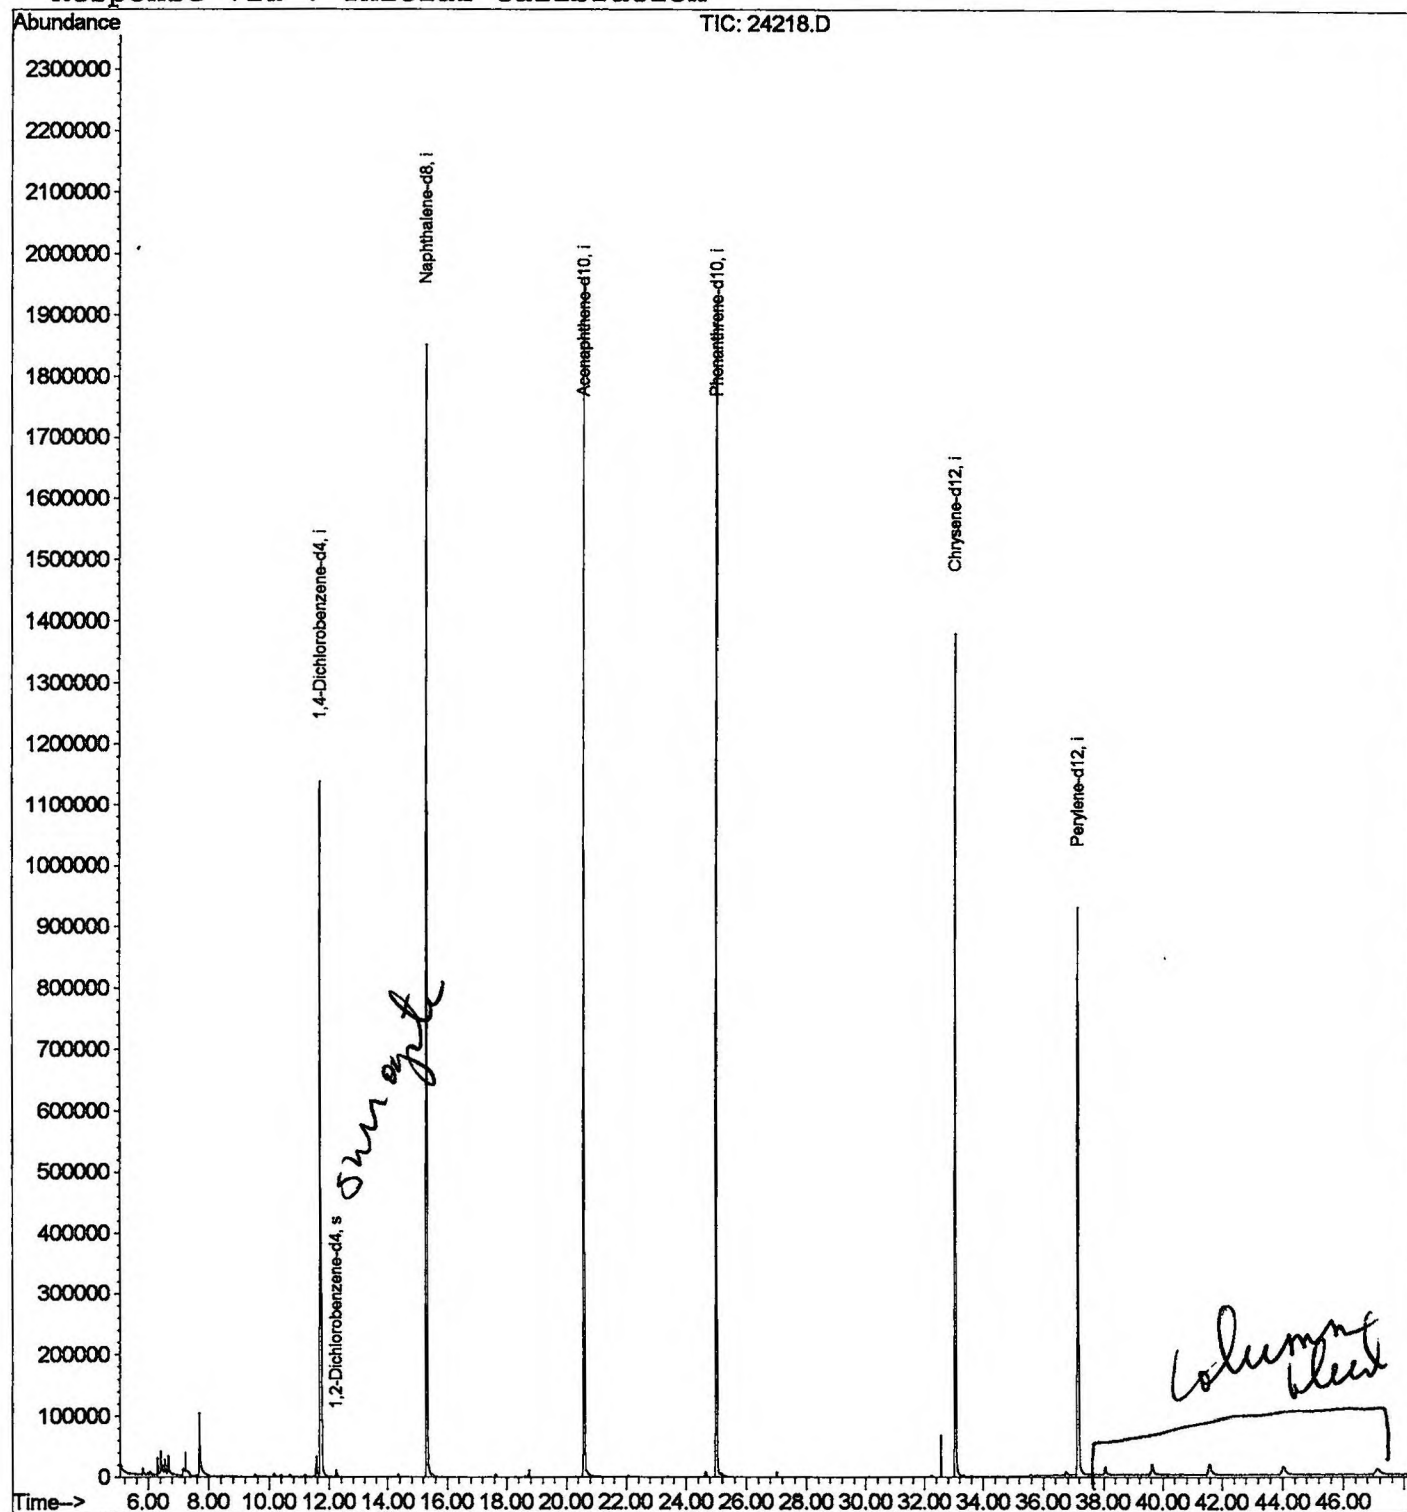

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\NOV0101\24218.D

Acq On : 1 Nov 2001 6:55 pm

Sample : gc/ms unknown

Misc :

MS Integration Params: LSCINT.P

Vial: 5

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	6.318	135	139	146	rBV	28284	58782	1.39%	0.265%
2	6.428	147	151	161	rVV	39281	118866	2.80%	0.536%
3	6.557	161	165	173	rVV	25231	65952	1.56%	0.298%
4	6.667	174	177	193	rVB	31400	82049	1.94%	0.370%
5	7.695	285	289	295	rBV	103192	254926	6.01%	1.150%
6	11.579	706	712	721	rBV	32367	78993	1.86%	0.356%
7	11.716	721	727	750	rVV	1138411	2977498	70.24%	13.434%
8	15.315	1114	1119	1137	rBV	1850697	4090304	96.49%	18.455%
9	20.594	1688	1694	1715	rBV	1961653	4239250	100.00%	19.127%
10	25.019	2169	2176	2189	rBV2	1921956	4046722	95.46%	18.259%
11	33.061	3045	3052	3071	rBV2	1379762	3267790	77.08%	14.744%
12	37.155	3489	3498	3512	rBV	928885	2549467	60.14%	11.503%
13	38.064	3589	3597	3602	rBV4	12668	46772	1.10%	0.211%
14	39.634	3759	3768	3779	rBV4	17368	87143	2.06%	0.393%
15	41.580	3969	3980	3987	rBV3	18276	101321	2.39%	0.457%
16	44.031	4235	4247	4258	rBV7	13026	97471	2.30%	0.440%




Sum of corrected areas: 22163306

24218.D NP103001.M

Tue Nov 06 11:48:23 2001

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\NOV0101\24218.D
Operator : 209 GALOS
Acquired : 1 Nov 2001 6:55 pm using AcqMethod NP101901
Instrument : GC/MS 209
Sample Name: gc/ms unknown
Misc Info :
Vial Number: 5
Quant File :NP101901.RES (RTE Integrator)

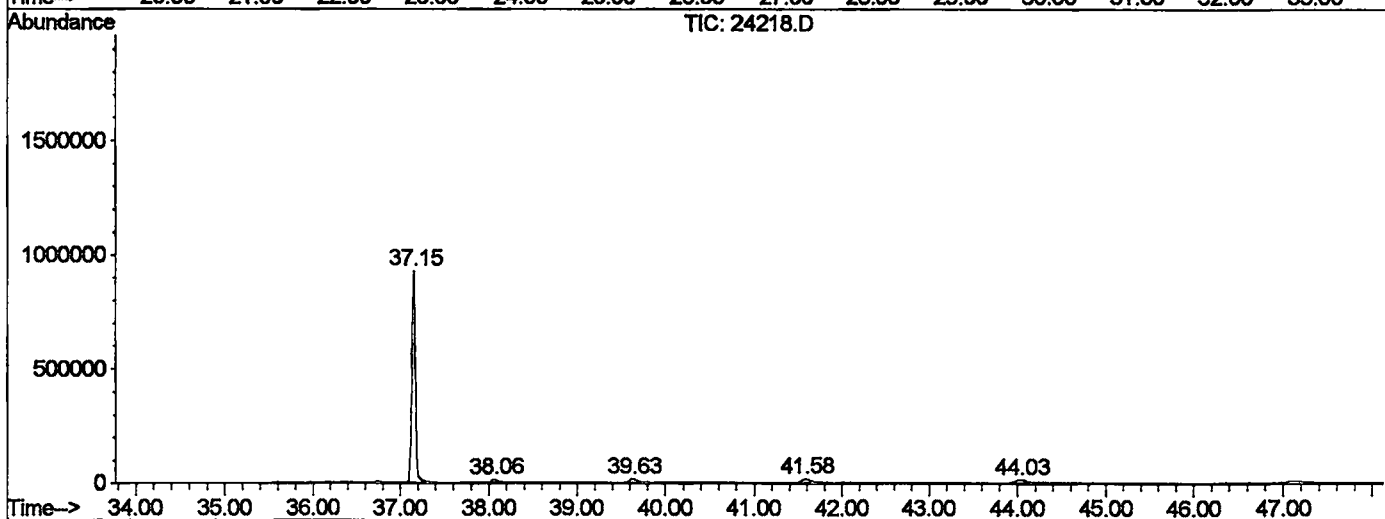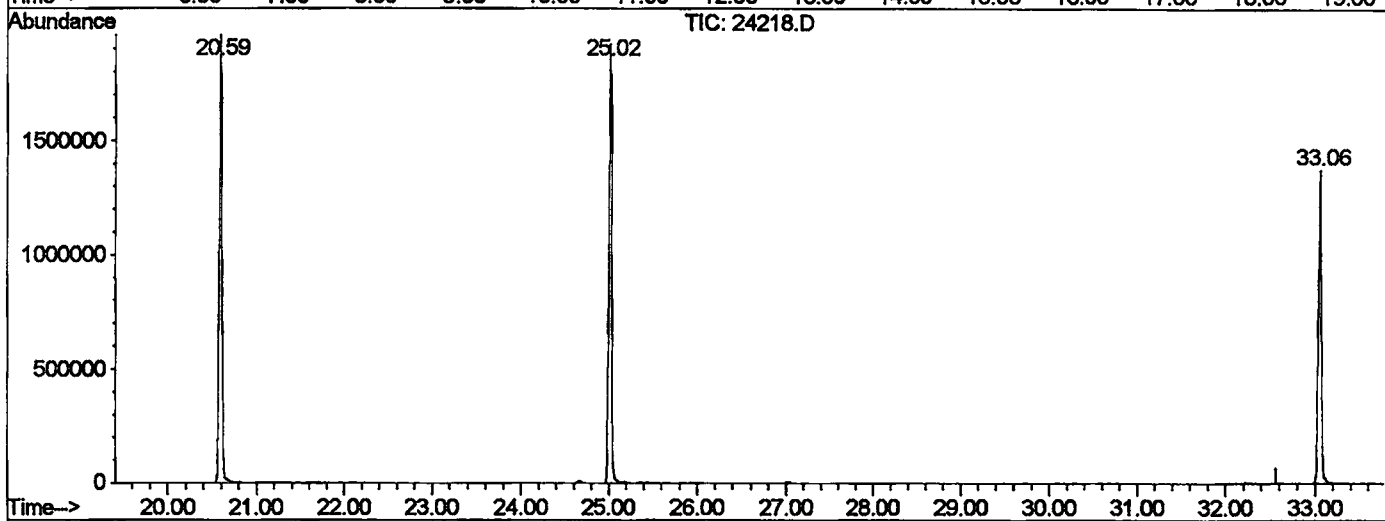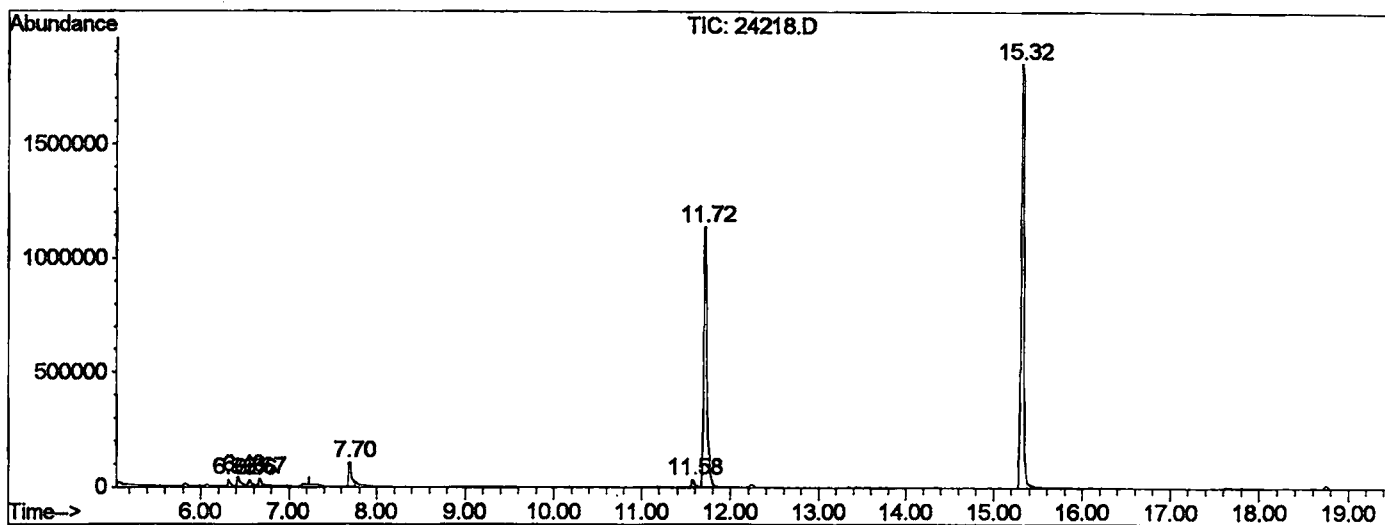

24218.D NP103001.M Tue Nov 06 11:48:26 2001

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\NOV0101\24218.D
 Acq On : 1 Nov 2001 6:55 pm
 Sample : gc/ms unknown
 Misc :
 MS Integration Params: LSCINT.P


Vial: 5
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\NP101901.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 2-Hexanone Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.43	0.80 ug/l	118866	1,4-Dichlorobenzene-d4	11.72

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Hexanone	100	C6H12O	000591-78-6	91
2		Methyl Isobutyl Ketone	100	C6H12O	000108-10-1	58
3		2-Hexanone, 4-hydroxy-5-methyl-3-pr	172	C10H20O2	061141-74-0	36
4		Propanal	58	C3H6O	000123-38-6	9

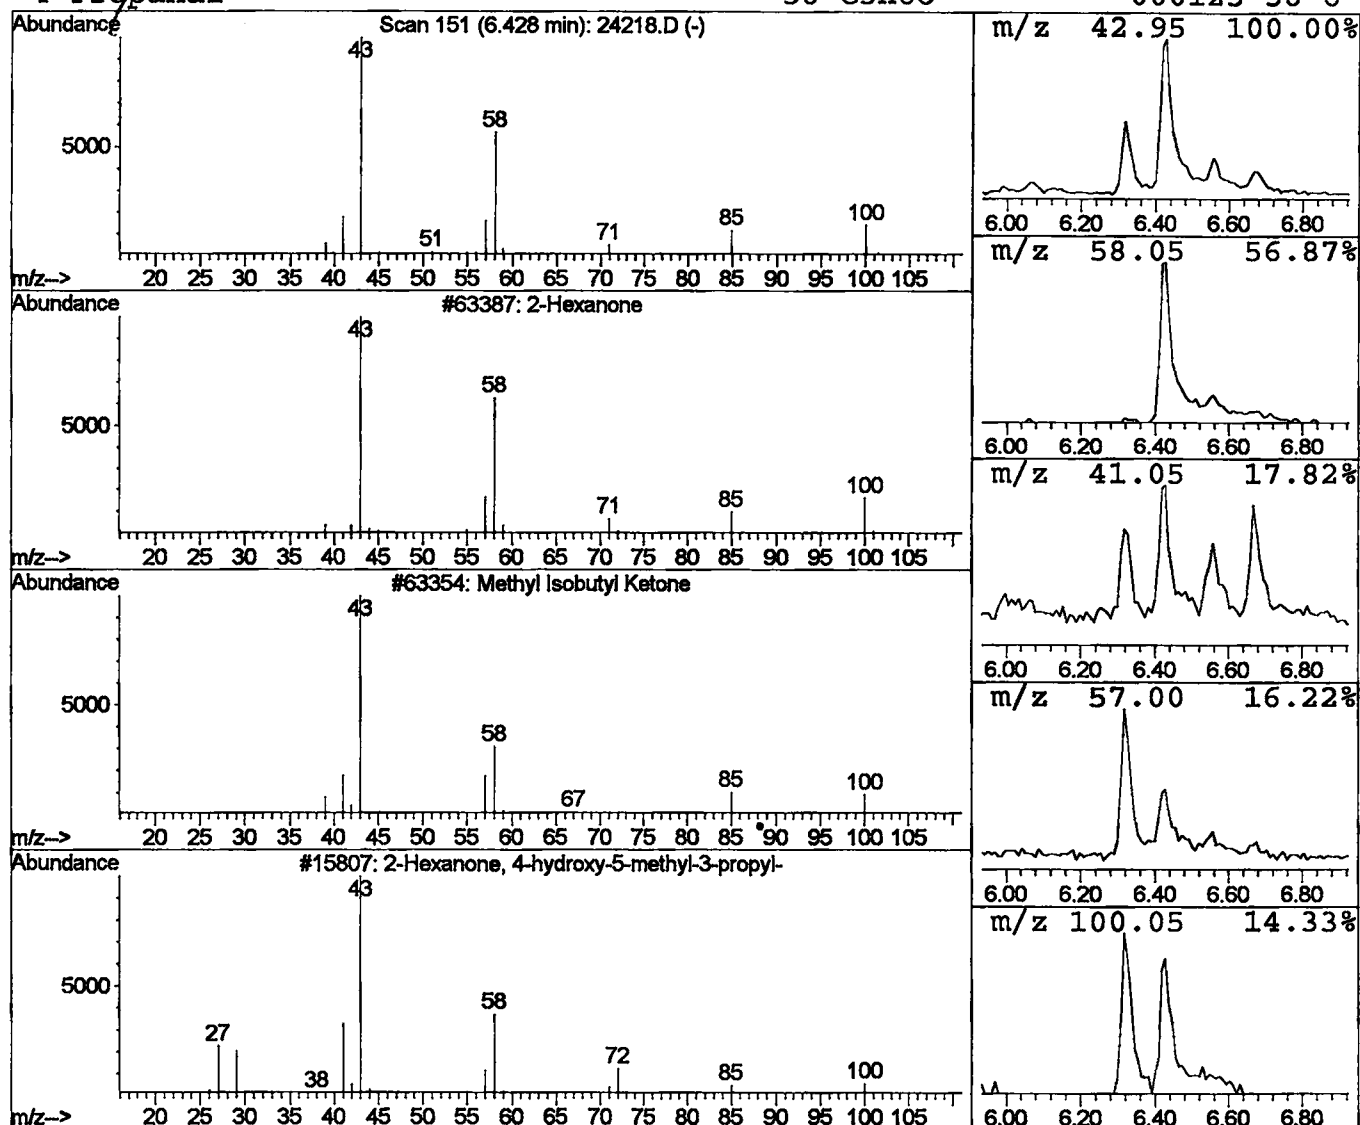

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\NOV0101\24218.D
Acq On : 1 Nov 2001 6:55 pm
Sample : gc/ms unknown
Misc :
MS Integration Params: LSCINT.P


Vial: 5
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\NP101901.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 2 3-Hexanol Concentration Rank 8

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.56	0.44 ug/l	65952	1,4-Dichlorobenzene-d4	11.72

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Hexanol		102	C6H14O	000623-37-0	83
2	3-Pentanol		88	C5H12O	000584-02-1	42
3	3-Pentanol, 2-methyl-		102	C6H14O	000565-67-3	36
4	Silane, trimethyl-		74	C3H10Si	000993-07-7	33

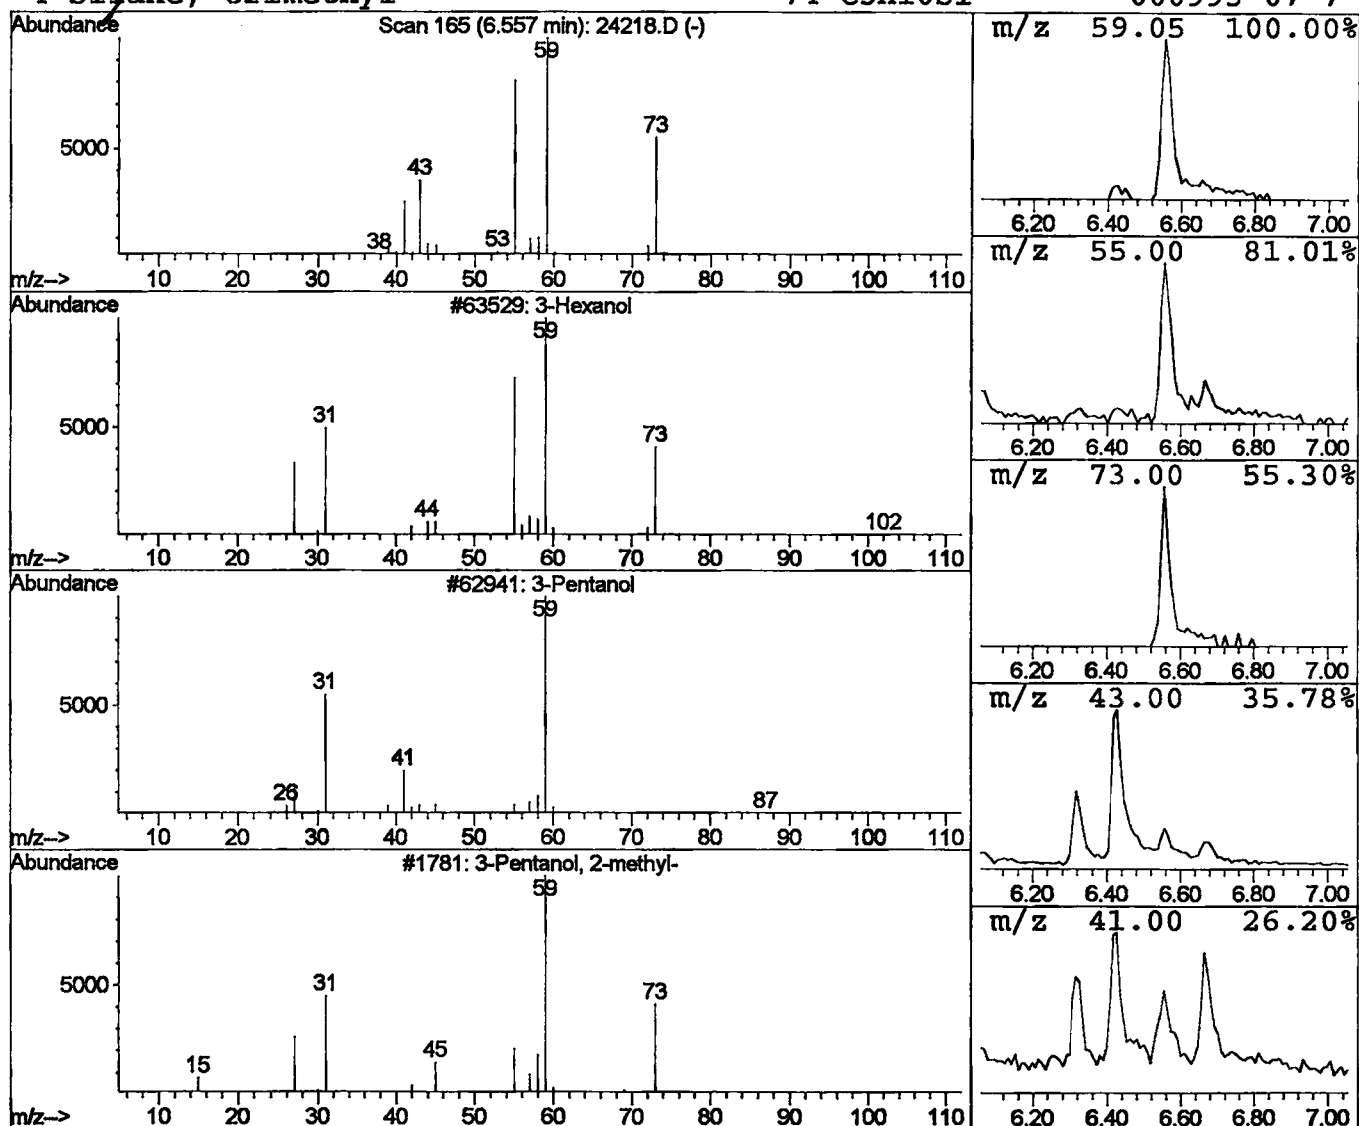

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\NOV0101\24218.D
 Acq On : 1 Nov 2001 6:55 pm
 Sample : gc/ms unknown
 Misc :
 MS Integration Params: LSCINT.P


Vial: 5
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\NP101901.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 3 2-Hexanol Concentration Rank 6

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.67	0.55 ug/l	82049	1,4-Dichlorobenzene-d4	11.72

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Hexanol	102	C6H14O	000626-93-7	83	
2	2-Pentanol, 4-methyl-	102	C6H14O	000108-11-2	74	
3	2-Butanol	74	C4H10O	000078-92-2	50	
4	2-Butanol, (R)-	74	C4H10O	014898-79-4	45	

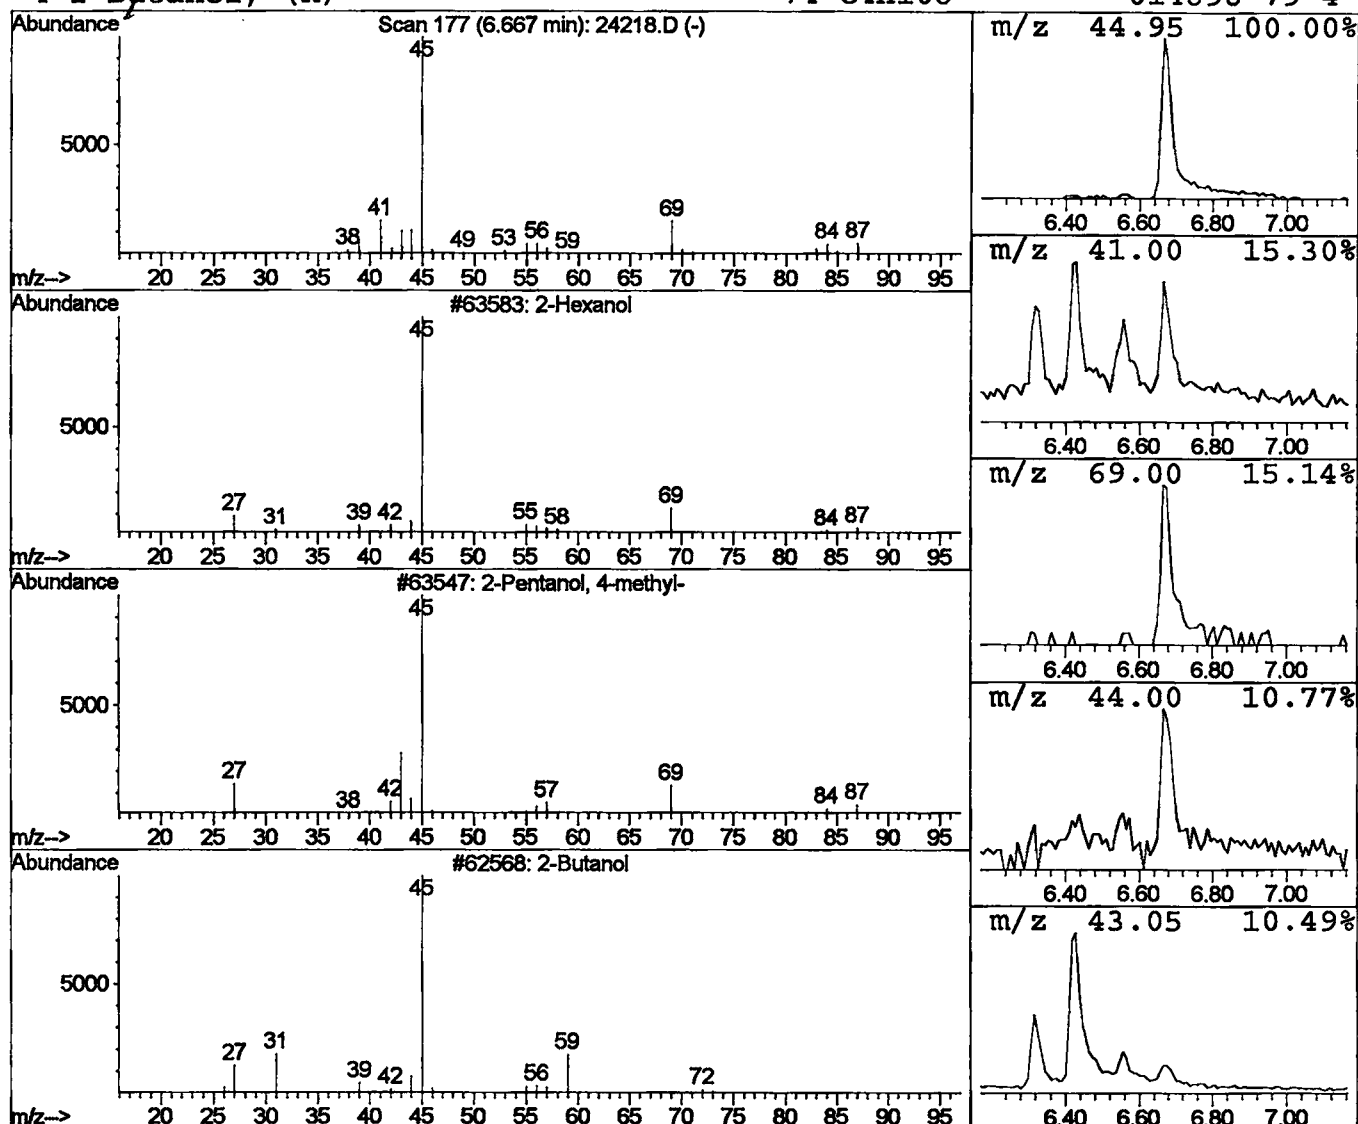

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\NOV0101\24218.D
 Acq On : 1 Nov 2001 6:55 pm
 Sample : gc/ms unknown
 Misc :
 MS Integration Params: LSCINT.P


Vial: 5
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\NP101901.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 4 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.70	1.71 ug/l	254926	1,4-Dichlorobenzene-d4	11.72

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	53	
2	Acetic acid, 1,1-dimethylethyl este	116	C6H12O2	000540-88-5	33	
3	Propanal, 2-hydroxy-2-methyl-	88	C4H8O2	020818-81-9	28	
4	Acetone	58	C3H6O	000067-64-1	9	

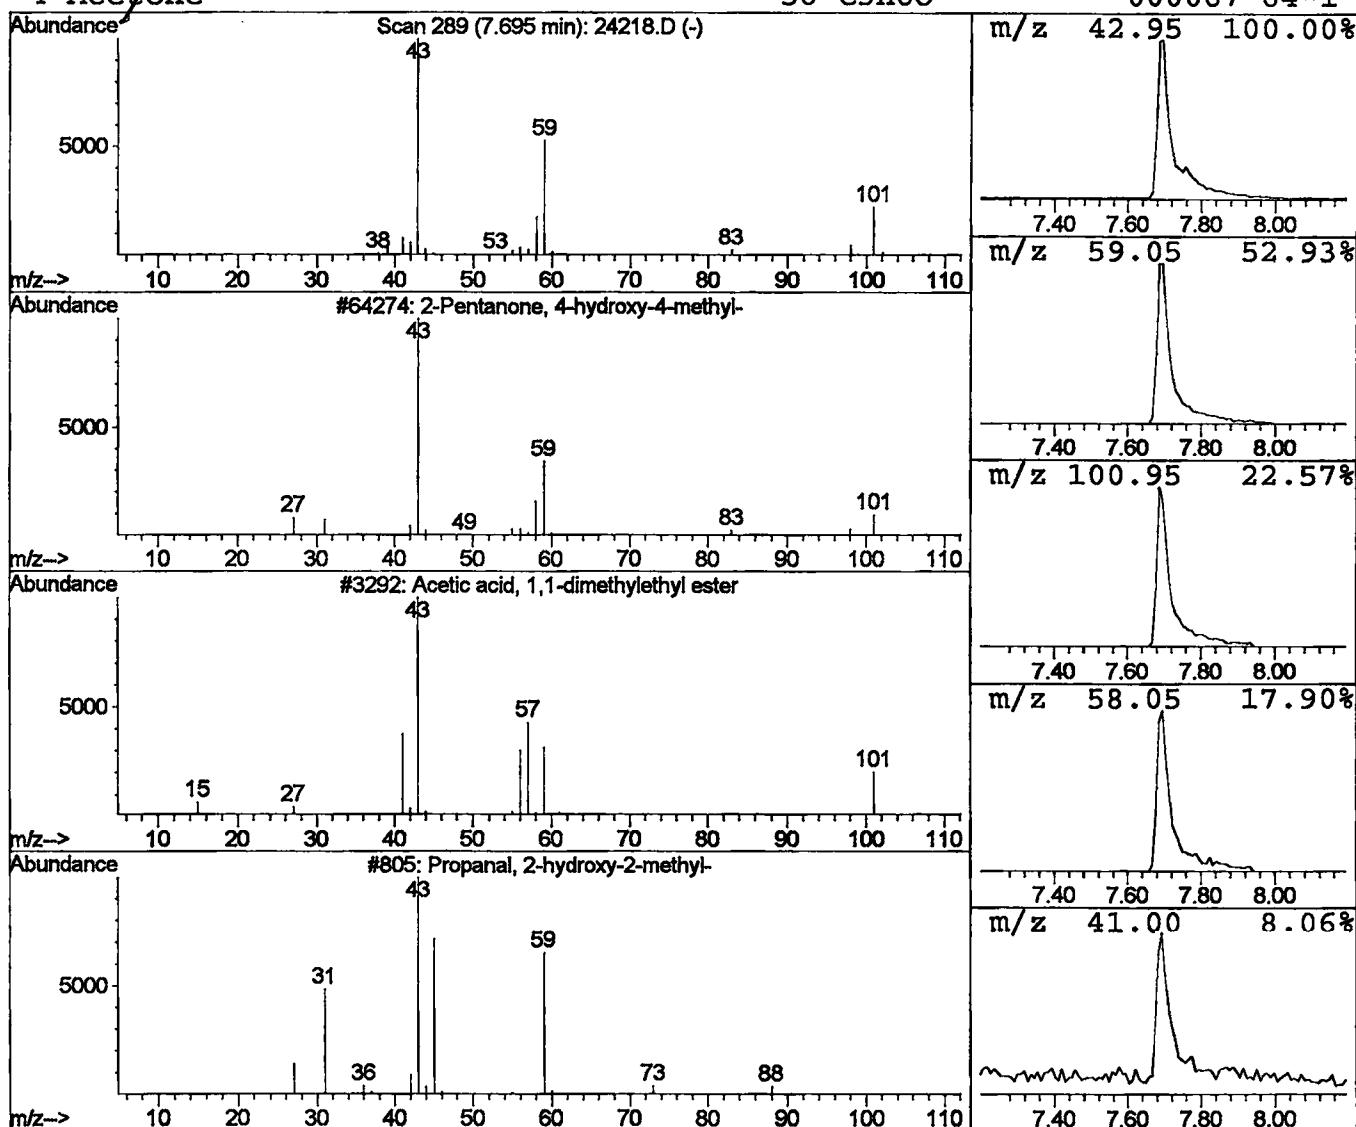

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\NOV0101\24218.D
Acq On : 1 Nov 2001 6:55 pm
Sample : gc/ms unknown
Misc :
MS Integration Params: LSCINT.P


Vial: 5
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\NP101901.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 5 1,4-Dichlorobenzene-d4 Concentration Rank 7

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.58	0.53 ug/l	78993	1,4-Dichlorobenzene-d4	11.72

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1,4-Dichlorobenzene-d4	150	C6Cl2D4	003855-82-1	53	
2	Benzene-1,2,3,4-d4-, 5,6-dichloro-	150	C6Cl2D4	002199-69-1	25	
3	Benzaldehyde, 2-hydroxy-3-methoxy-	152	C8H8O3	000148-53-8	10	
4	((3-Ethoxyphenyl)-1-methanol	152	C9H12O2	000000-00-0	9	

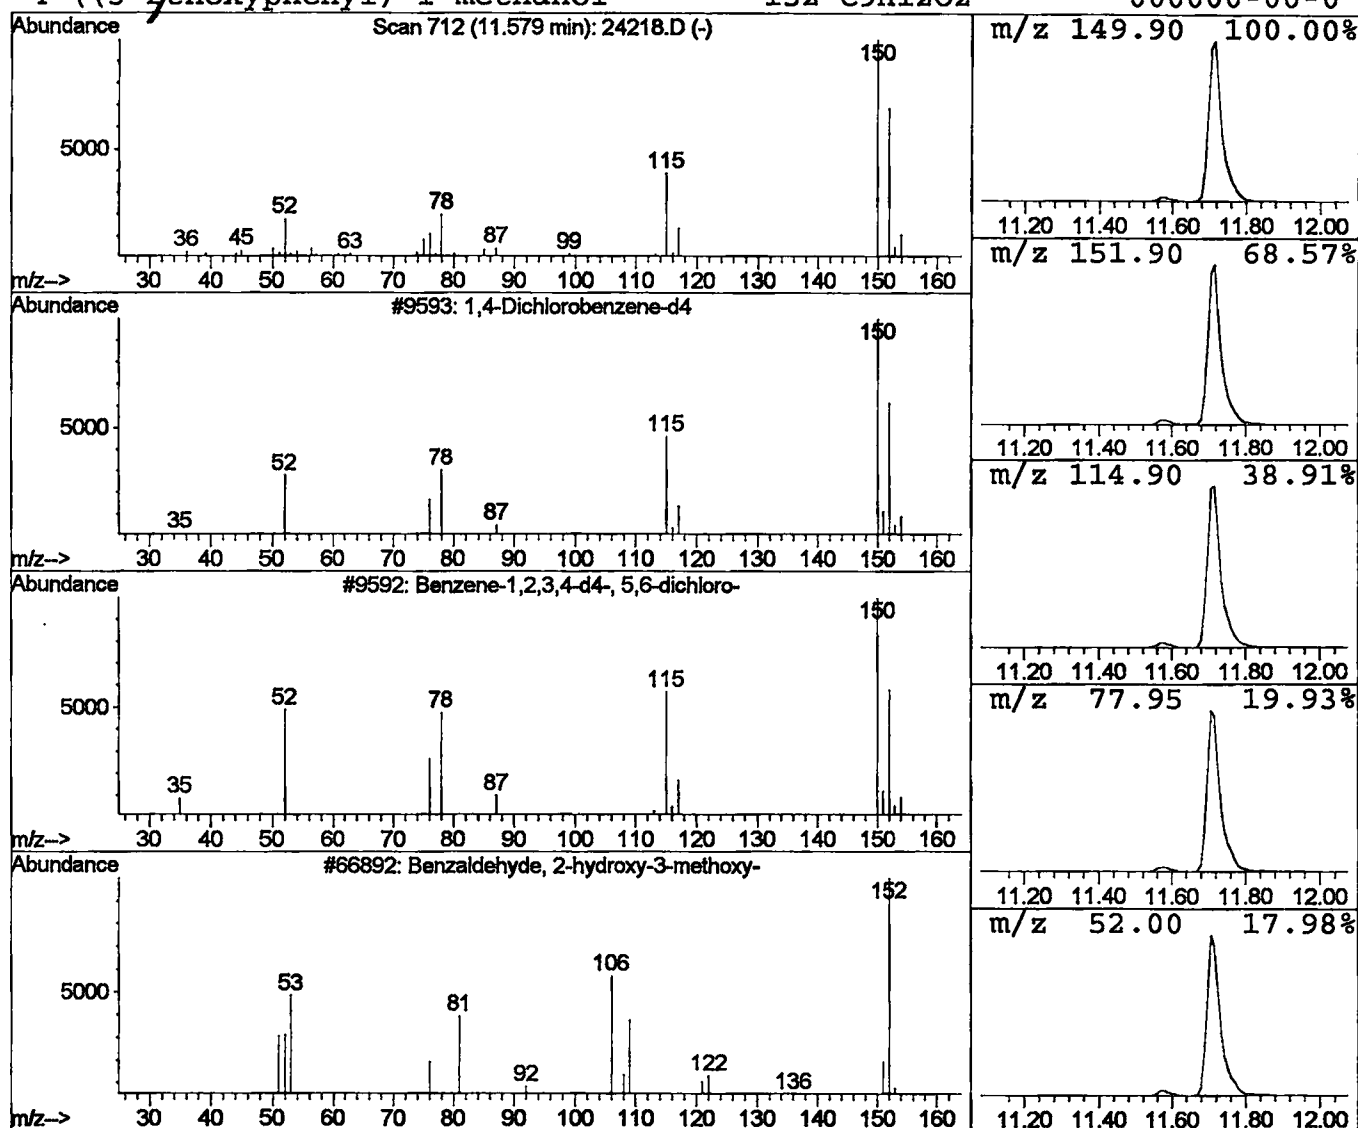

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\NOV0101\24218.D
Acq On : 1 Nov 2001 6:55 pm
Sample : gc/ms unknown
Misc :
MS Integration Params: LSCINT.P










Vial: 5
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\NP101901.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 6 Mercaptoacetic acid, bis(trimethylsilyl) Concentration Rank 5

R.T.	EstConc	Area	Relative to ISTD	R.T.
39.63	0.68 ug/l	87143	Perylene-d12	37.16

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Mercaptoacetic acid, bis(trimethylsilyl)	236	C8H20O2SSi2	006398-62-5	32
2			3,7-Dioxo-2,8-disilanonane, 2,2,8,8	220	C9H24O2Si2	017887-80-8	27
3			3,6-Dioxo-2,4,5,7-tetrasilaoctane,	294	C10H30O2Si4	004342-25-0	17
4			Ethanedioic acid, bis(trimethylsilyl)	234	C8H18O4Si2	018294-04-7	17

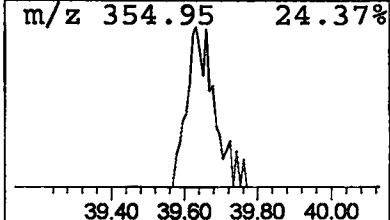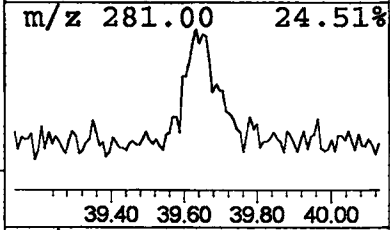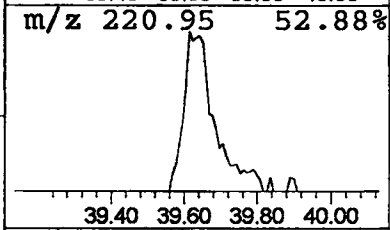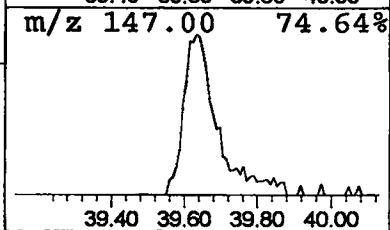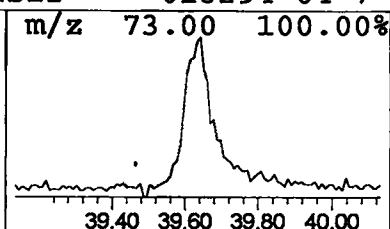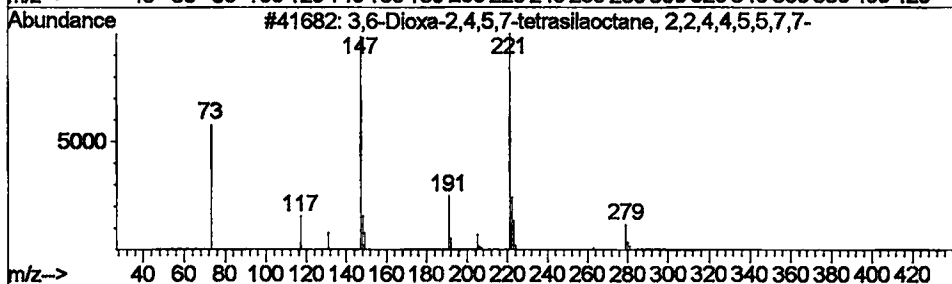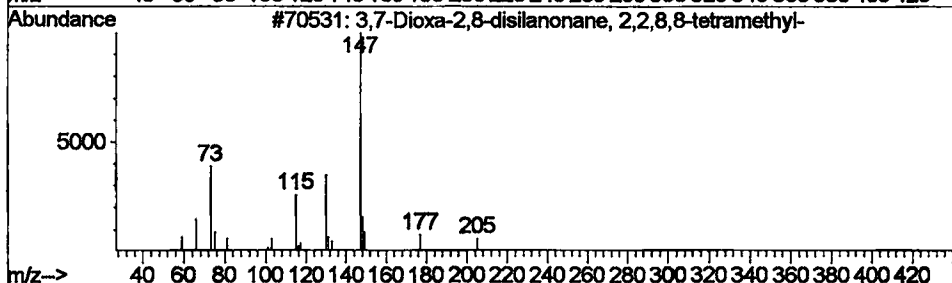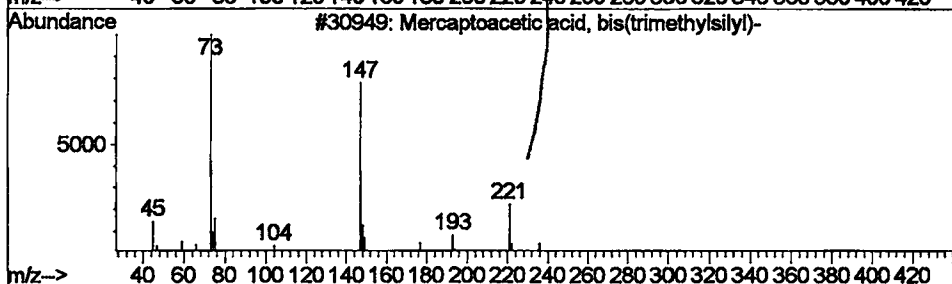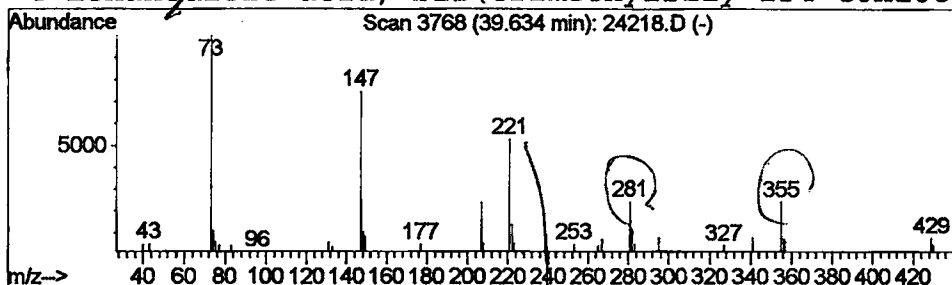

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\NOV0101\24218.D
Acq On : 1 Nov 2001 6:55 pm
Sample : gc/ms unknown
Misc :
MS Integration Params: LSCINT.P

Vial: 5
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00


Quant Method : C:\HPCHEM\1\METHODS\NP101901.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 7 3,6-Dioxa-2,4,5,7-tetrasilaoct Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
41.58	0.79 ug/l	101321	Perylene-d12	37.16

Column bleed

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3,6-Dioxa-2,4,5,7-tetrasilaoctane,	294	C10H30O2Si4	004342-25-0	47
2		Mercaptoacetic acid, bis(trimethyls	236	C8H20O2SSi2	006398-62-5	23
3		Pentanoic acid, 2-[(trimethylsilyl)	262	C11H26O3Si2	055887-46-2	16
4		Ethanedioic acid, bis(trimethylsily	234	C8H18O4Si2	018294-04-7	16

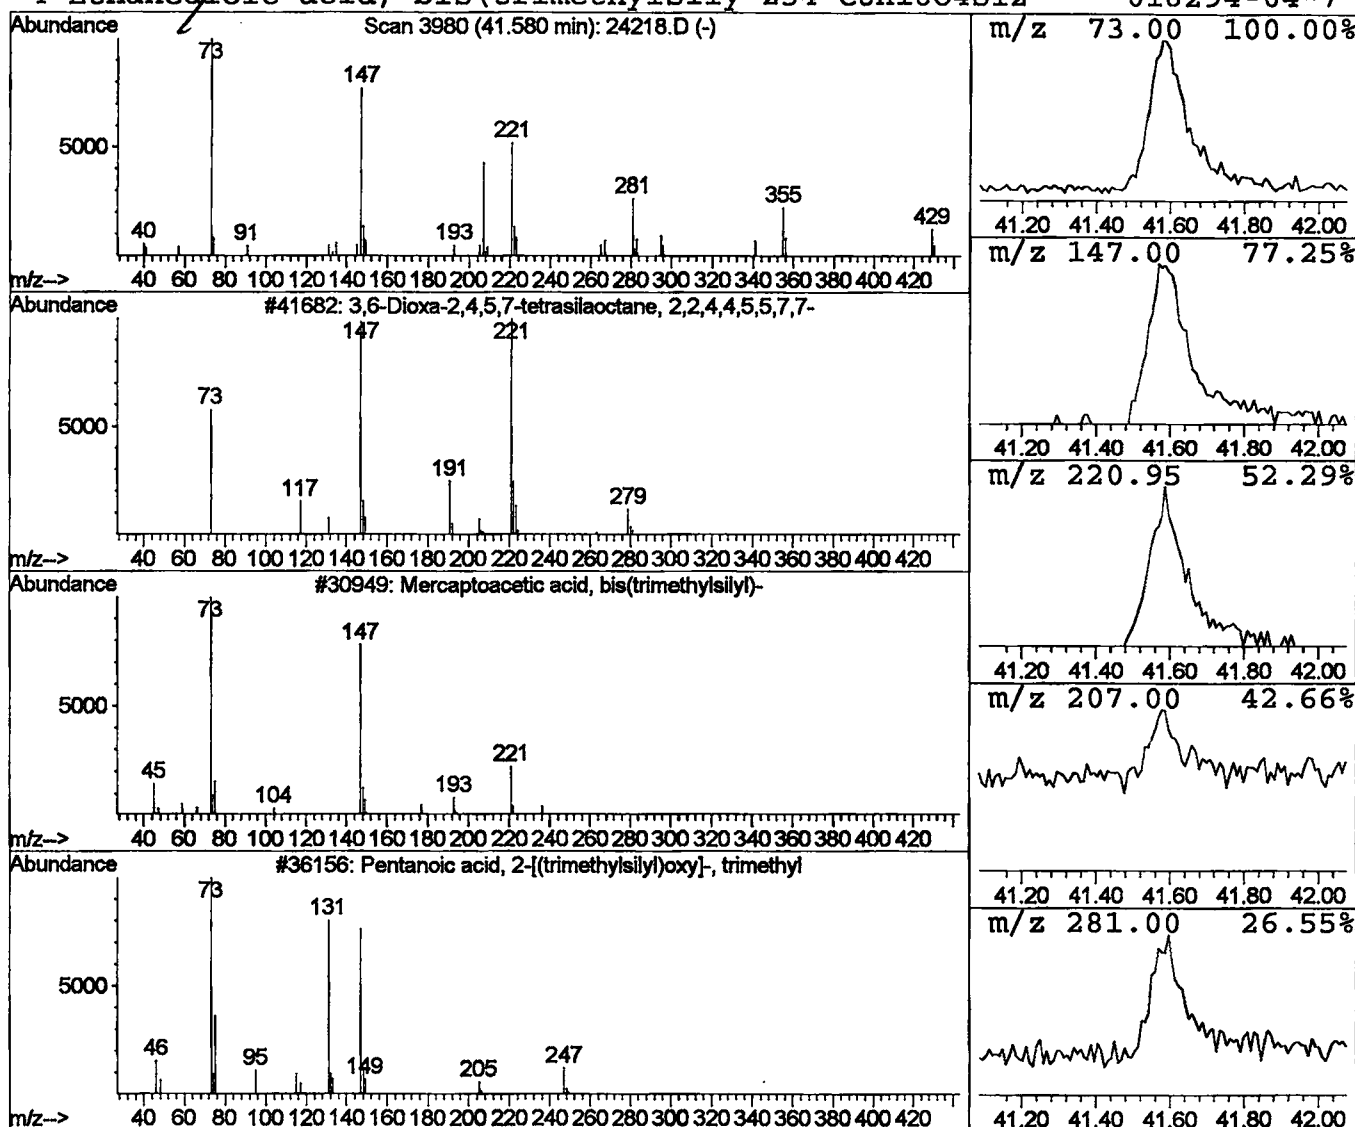

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\NOV0101\24218.D
Acq On : 1 Nov 2001 6:55 pm
Sample : gc/ms unknown
Misc :
MS Integration Params: LSCINT.P


Vial: 5
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\NP101901.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 8 3,6-Dioxa-2,4,5,7-tetrasilaoct Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
44.03	0.76 ug/l	97471	Perylene-d12	37.16

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	3,6-Dioxa-2,4,5,7-tetrasilaoctane,	294	C10H30O2Si4	004342-25-0	38	
2	Acetic acid, [(1,3-dihydro-1,3-diox	267	C11H9NO5S	042300-59-4	22	
3	Mercaptoacetic acid, bis(trimethyls	236	C8H20O2SSi2	006398-62-5	17	
4	1,2-Benzenedicarboxylic acid, bis(t	310	C14H22O4Si2	002078-22-0	17	

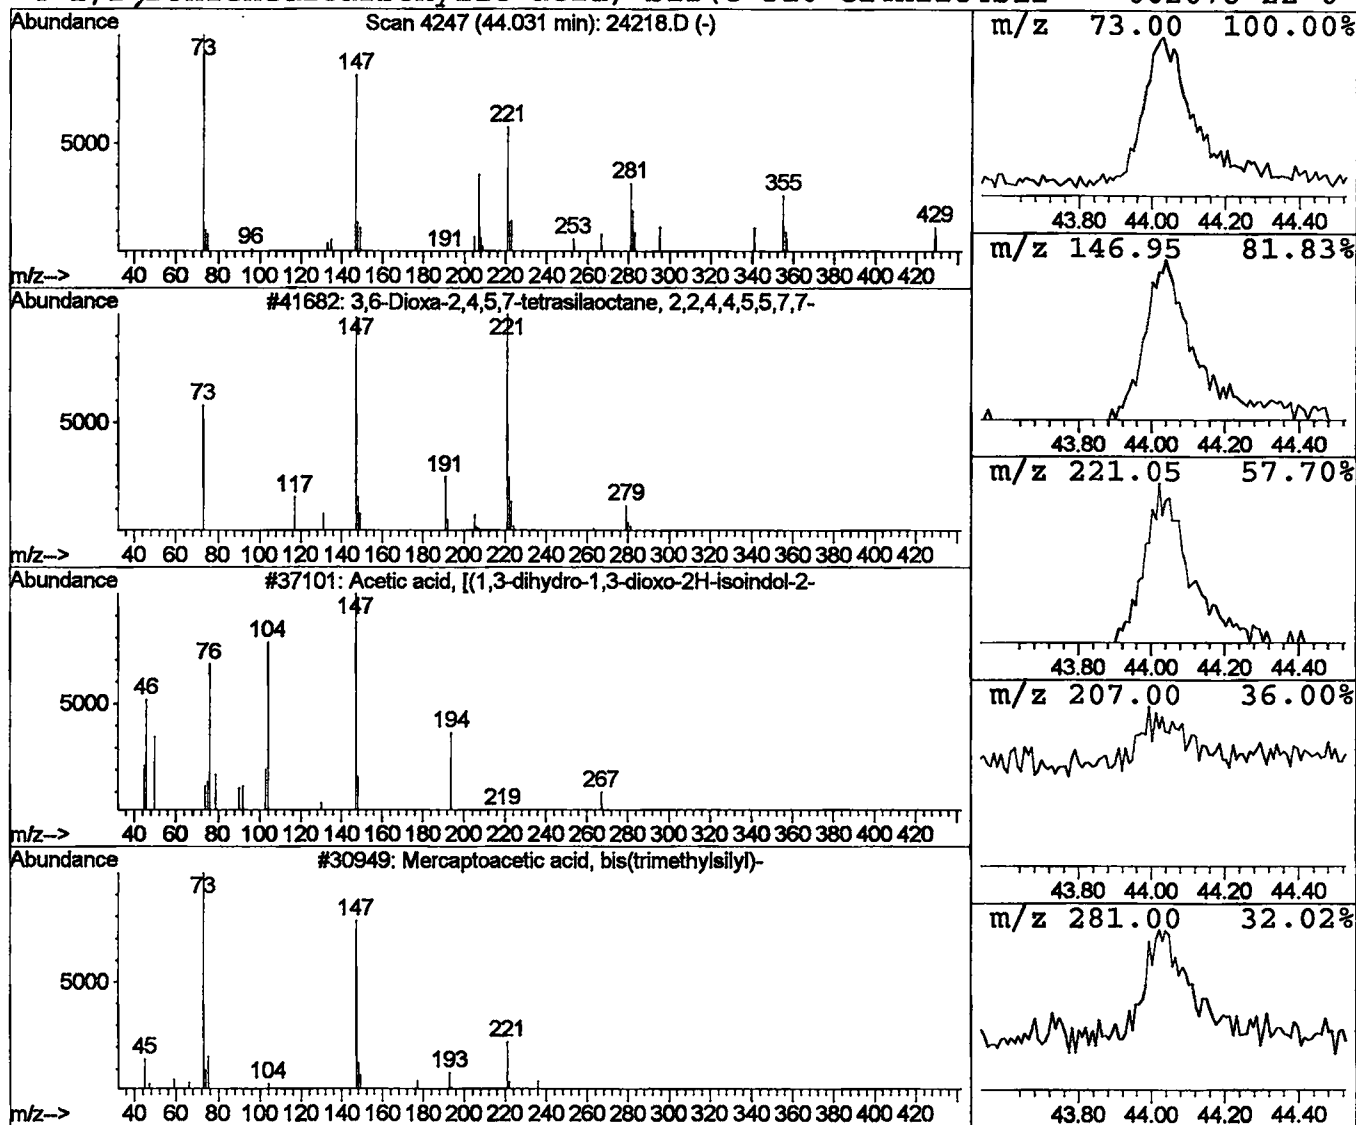

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 1 Nov 2001 6:55 pm
 Data File: C:\HPCHEM\1\DATA\NOV0101\24218.D
 Name: gc/ms unknown
 Misc:
 Method: C:\HPCHEM\1\METHODS\NP101901.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc Units	Area	IntStd	ISRT	ISArea	ISConc
2- Hexanone	6.43	0.8 ug/l	118866	ISTD01	11.72	2977500	20.0
3- Hexanol	6.56	0.4 ug/l	65952	ISTD01	11.72	2977500	20.0
2- Hexanol	6.67	0.6 ug/l	82049	ISTD01	11.72	2977500	20.0
2-Pentanone, 4-hydro	7.70	1.7 ug/l	254926	ISTD01	11.72	2977500	20.0
1,4-Dichlorobenzene-	11.58	0.5 ug/l	78993	ISTD01	11.72	2977500	20.0
Mercaptoacetic acid,	39.63	0.7 ug/l	87143	ISTD06	37.16	2549470	20.0
3,6-Dioxo-2,4,5,7-te	41.58	0.8 ug/l	101321	ISTD06	37.16	2549470	20.0
3,6-Dioxo-2,4,5,7-te	44.03	0.8 ug/l	97471	ISTD06	37.16	2549470	20.0

24218.D NP103001.M Tue Nov 06 11:48:45 2001

Comments for Sample AD24218 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 11-07-2001 Time: 14:55:02

A scan of the extract prepared for the 508 analysis, from 35-550 amu using a mass spectrometer, does not reveal the presence of non-target compounds. However, 1,2-Dichlorobenzene-d4 is present at 0.28 ug/L, probably due to laboratory contamination since it is a Surrogate Standard used in GCMS methods. Also present are some siloxanes associated with column bleed.