

User: Galos, Marie
 Westchester Dept. of Labs & Research
 Date: 11/07/2001 Time: 15:04:42

Sample: AD24430
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 11/7/01 14:50 Ended: 11/7/01 14:50 Analyst: MG
 Page: 1

	Component Name	Vol	Result
1	Other unknown compounds		see comment

Comments for Sample AD24430 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Galos, Marie

Date: 11-07-2001 Time: 15:05:11

A scan of the extract prepared for the 508 analysis, from 35-550 amu using a mass spectrometer, does not reveal the presence of non-target compounds.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV0201\24430.D
 Acq On : 2 Nov 2001 9:52 pm
 Sample : gc/ms unknown
 Misc :
 MS Integration Params: RTEINT.P
 Quant Time: Nov 5 12:09 2001

Vial: 8
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: NP103001.RES

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Fri Nov 02 16:41:16 2001
 Response via : Initial Calibration
 DataAcq Meth : NP103001

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	11.71	152	553093	20.00	ug/l	-0.01
19) Naphthalene-d8	15.32	136	2126867m	20.00	ug/l	-0.01
31) Acenaphthene-d10	20.60	164	1035382	20.00	ug/l	-0.01
49) Phenanthrene-d10	25.01	188	1538471	20.00	ug/l	-0.02
59) Chrysene-d12	33.06	240	1102172	20.00	ug/l	-0.01
68) Perylene-d12	37.15	264	799381	20.00	ug/l	-0.01

System Monitoring Compounds

4) 2-Fluorophenol	0.00	112	0	0.00	ug/l	
Spiked Amount 75.000			Recovery	=	0.00%	
5) Phenol-d5	0.00	99	0	0.00	ug/l	
Spiked Amount 75.000			Recovery	=	0.00%	
6) 2-Chlorophenol-d4	11.70	132	432	0.01	ug/l	0.46
Spiked Amount 75.000			Recovery	=	0.01%	
7) 1,2-Dichlorobenzene-d4	12.24	152	6629	0.26	ug/l	-0.01
Spiked Amount 50.000			Recovery	=	0.52%	
20) Nitrobenzene-d5	0.00	82	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
32) 2-Fluorobiphenyl	18.74	172	1941	0.03	ug/l	0.13
Spiked Amount 50.000			Recovery	=	0.06%	
33) 2,4,6-Tribromophenol	0.00	330	0	0.00	ug/l	
Spiked Amount 75.000			Recovery	=	0.00%	
62) Terphenyl-d14	0.00	244	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	

Target Compounds

					Qvalue
2) Pyridine	0.00	79	0	N.D.	
3) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
8) Phenol	0.00	94	0	N.D.	
9) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
10) 2-Chlorophenol	0.00	128	0	N.D.	
11) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
12) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
13) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
14) 2-Methylphenol	0.00	108	0	N.D.	
15) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
16) 3&4-Methylphenol	0.00	108	0	N.D.	
17) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
18) Hexachloroethane	0.00	117	0	N.D.	
21) Nitrobenzene	0.00	77	0	N.D.	
22) Isophorone	0.00	82	0	N.D.	

(#) = qualifier out of range (m) = manual integration
 24430.D NP103001.M Mon Nov 05 12:10:11 2001

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV0201\24430.D
 Acq On : 2 Nov 2001 9:52 pm
 Sample : gc/ms unknown
 Misc :
 MS Integration Params: RTEINT.P
 Quant Time: Nov 5 12:09 2001

Vial: 8
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: NP103001.RES

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Fri Nov 02 16:41:16 2001
 Response via : Initial Calibration
 DataAcq Meth : NP103001

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
23) 2-Nitrophenol	0.00	139	0	N.D.		
24) 2,4-Dimethylphenol	0.00	107	0	N.D.		
25) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.		
26) 2,4-Dichlorophenol	0.00	162	0	N.D.		
27) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.		
28) Naphthalene	0.00	128	0	N.D.		
29) Hexachlorobutadiene	0.00	225	0	N.D.		
30) 4-Chloro-3-methylphenol	0.00	107	0	N.D.		
34) Hexachlorocyclopentadiene	0.00	237	0	N.D.		
35) 2,4,6-Trichlorophenol	0.00	196	0	N.D.		
36) 2,4,5-Trichlorophenol	0.00	196	0	N.D.		
37) 2-Chloronaphthalene	0.00	162	0	N.D.		
38) Dimethylphthalate	0.00	163	0	N.D.		
39) 2,6-Dinitrotoluene	0.00	165	0	N.D.		
40) Acenaphthylene	0.00	152	0	N.D.		
41) Acenaphthene	0.00	153	0	N.D.		
42) 2,4-Dinitrophenol	0.00	184	0	N.D.		
43) 4-Nitrophenol	0.00	65	0	N.D.		
44) 2,4-Dinitrotoluene	0.00	165	0	N.D.		
45) Diethylphthalate	0.00	149	0	N.D.		
46) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.		
47) Fluorene	0.00	166	0	N.D.		
48) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.		
50) 4,6-Dinitro-2-methylphenol	0.00	198	0	N.D.		
51) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
52) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
53) Hexachlorobenzene	0.00	284	0	N.D.		
54) Pentachlorophenol	0.00	266	0	N.D.		
55) Phenanthrene	25.02	178	364	N.D.		
56) Anthracene	25.02	178	363	N.D.		
57) Di-n-butylphthalate	27.03	149	1684	N.D.		
58) Fluoranthene	0.00	202	0	N.D.		
60) 3,3'-Dichlorobenzidine	0.00	252	0	N.D.		
61) Benzidine	0.00	184	0	N.D.		
63) Pyrene	0.00	202	0	N.D.		
64) Butylbenzylphthalate	0.00	149	0	N.D.		
65) Benzo(a)anthracene	33.06	228	2831	N.D.		
66) Bis(2-ethylhexyl)phthalate	33.32	149	850	N.D.		
67) Chrysene	33.06	228	2831	N.D.		
69) Di-n-Octylphthalate	0.00	149	0	N.D.		
70) Benzo(b)fluoranthene	0.00	252	0	N.D.		

(#) = qualifier out of range (m) = manual integration

24430.D NP103001.M Mon Nov 05 12:10:16 2001

Page 2

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV0201\24430.D

Vial: 8

Acq On : 2 Nov 2001 9:52 pm

Operator: 209 GALOS

Sample : gc/ms unknown

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Nov 5 12:09 2001

Quant Results File: NP103001.RES

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Nov 02 16:41:16 2001

Response via : Initial Calibration

DataAcq Meth : NP103001

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
71) Benzo(k)fluoranthene	0.00	252	0	N.D.		
72) Benzo(a)pyrene	37.16	252	3167	N.D.		
73) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
74) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
75) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration
24430.D NP103001.M Mon Nov 05 12:10:17 2001

Page 3


Quantitation Report

Data File : C:\HPCHEM\1\DATA\NOV0201\24430.D
Acq On : 2 Nov 2001 9:52 pm
Sample : gc/ms unknown
Misc :
MS Integration Params: RTEINT.P
Quant Time: Nov 5 12:09 2001

Vial: 8
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: NP103001.RES

Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Fri Nov 02 16:41:16 2001
Response via : Initial Calibration

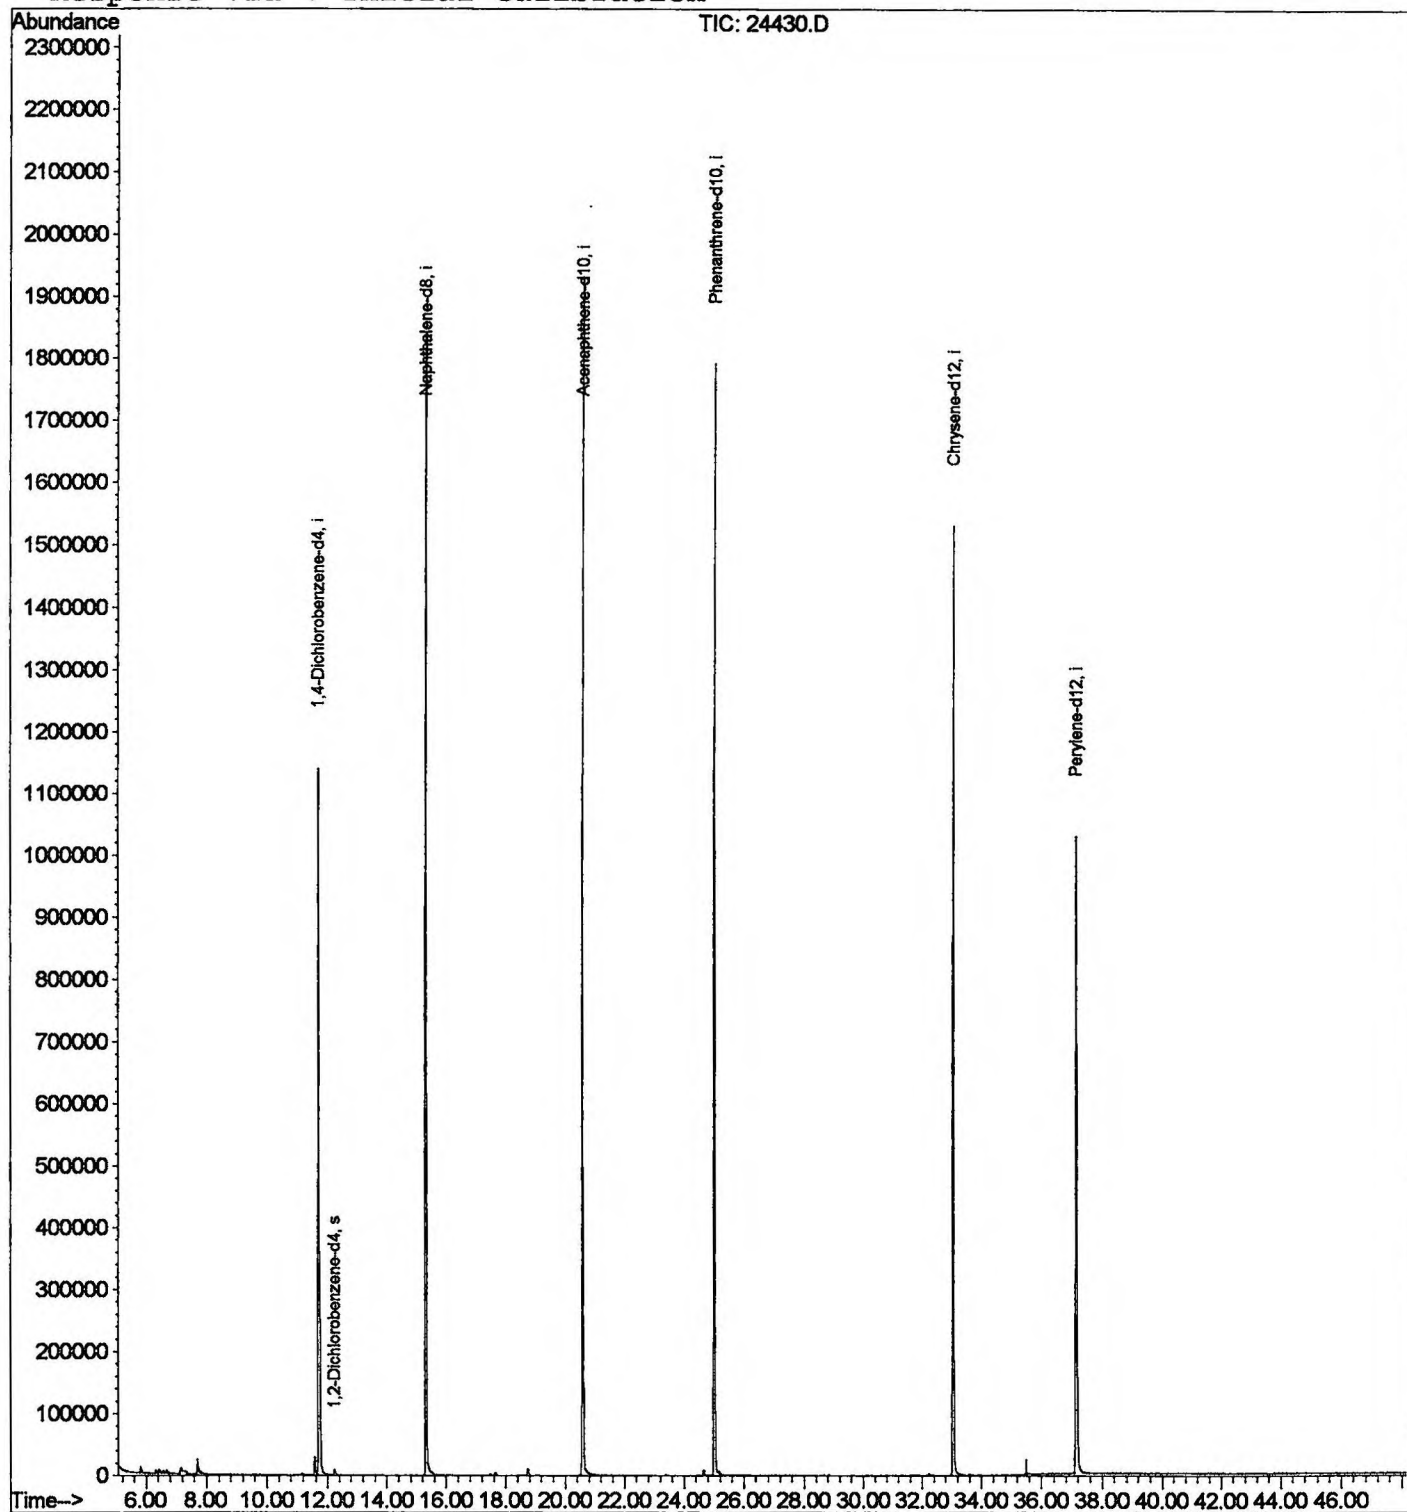

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\NOV0201\24430.D

Acq On : 2 Nov 2001 9:52 pm

Sample : gc/ms unknown

Misc :

MS Integration Params: LSCINT.P

Vial: 8

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	7.700	284	289	297	rBV	25731	73456	1.77%	0.340%
2	11.574	707	711	721	rBV	30491	76511	1.84%	0.354%
3	11.712	721	726	747	rVV	1139068	2909536	69.93%	13.450%
4	15.320	1113	1119	1136	rBV	1841639	3965730	95.32%	18.333%
5	20.598	1687	1694	1711	rBV	1931811	4160446	100.00%	19.233%
6	25.014	2168	2175	2188	rBV2	1792019	3964086	95.28%	18.325%
7	33.056	3044	3051	3068	rBV2	1530534	3520933	84.63%	16.277%
8	37.151	3490	3497	3512	rBV	1027007	2960964	71.17%	13.688%




Sum of corrected areas: 21631662

24430.D NP103001.M

Tue Nov 06 08:06:50 2001

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\NOV0201\24430.D
Operator : 209 GALOS
Acquired : 2 Nov 2001 9:52 pm using AcqMethod NP103001
Instrument : GC/MS 209
Sample Name: gc/ms unknown
Misc Info :
Vial Number: 8
Quant File :NP103001.RES (RTE Integrator)

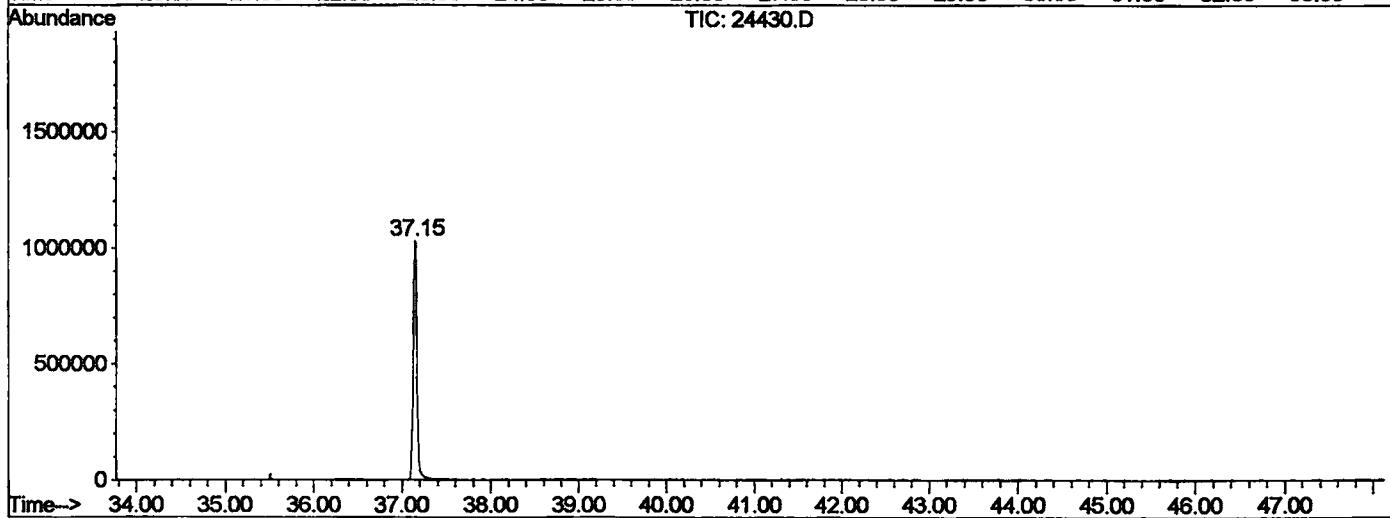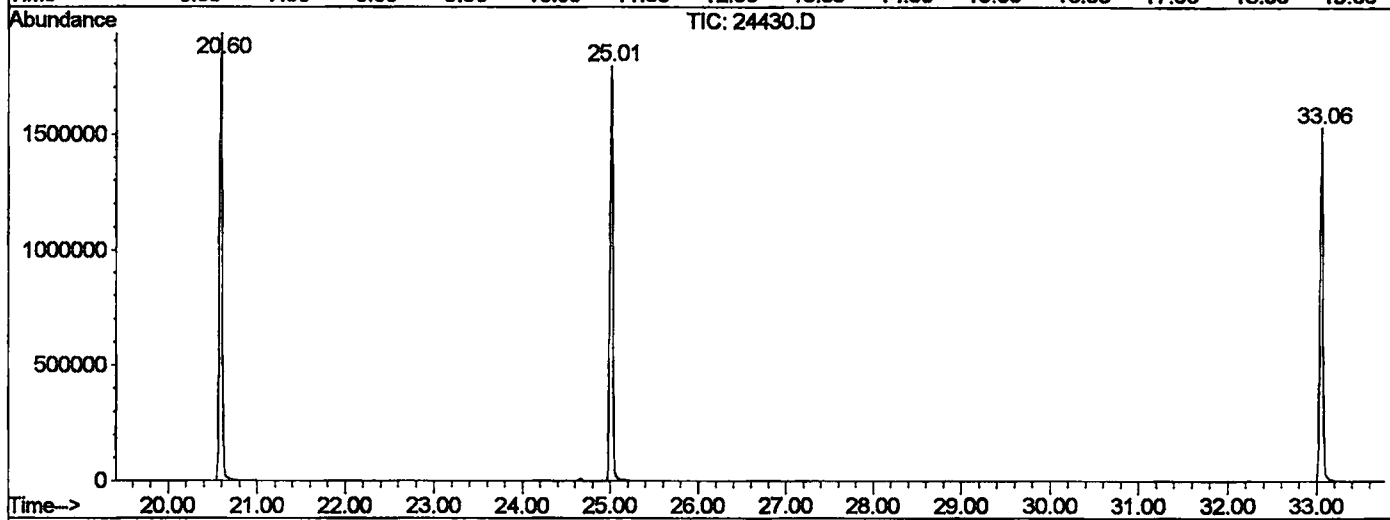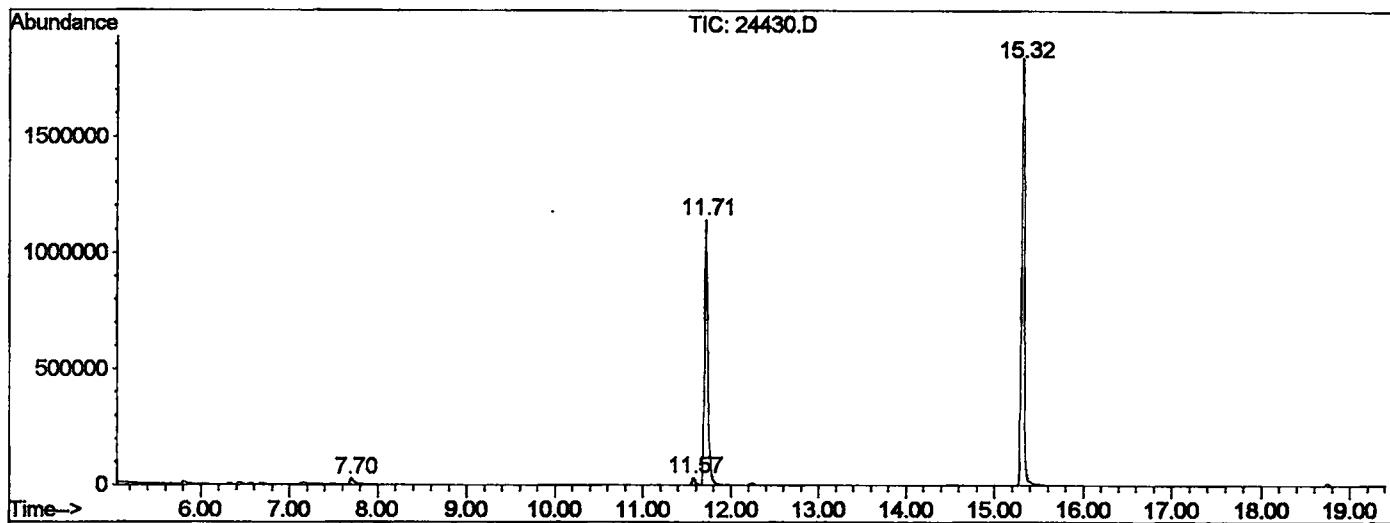

24430.D NP103001.M Tue Nov 06 08:06:52 2001

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\NOV0201\24430.D
Acq On : 2 Nov 2001 9:52 pm
Sample : gc/ms unknown
Misc :
MS Integration Params: LSCINT.P


Vial: 8
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 Acetic acid, 1,1-dimethylethyl Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.70	0.50 ug/l	73456	1,4-Dichlorobenzene-d4	11.71

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Acetic acid, 1,1-dimethylethyl este	116	C6H12O2	000540-88-5	50
2			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	42
3			Oxirane, (propoxymethyl)-	116	C6H12O2	003126-95-2	33
4			2-Pentanone, 5-(2-propynyloxy)-	140	C8H12O2	055702-70-0	17

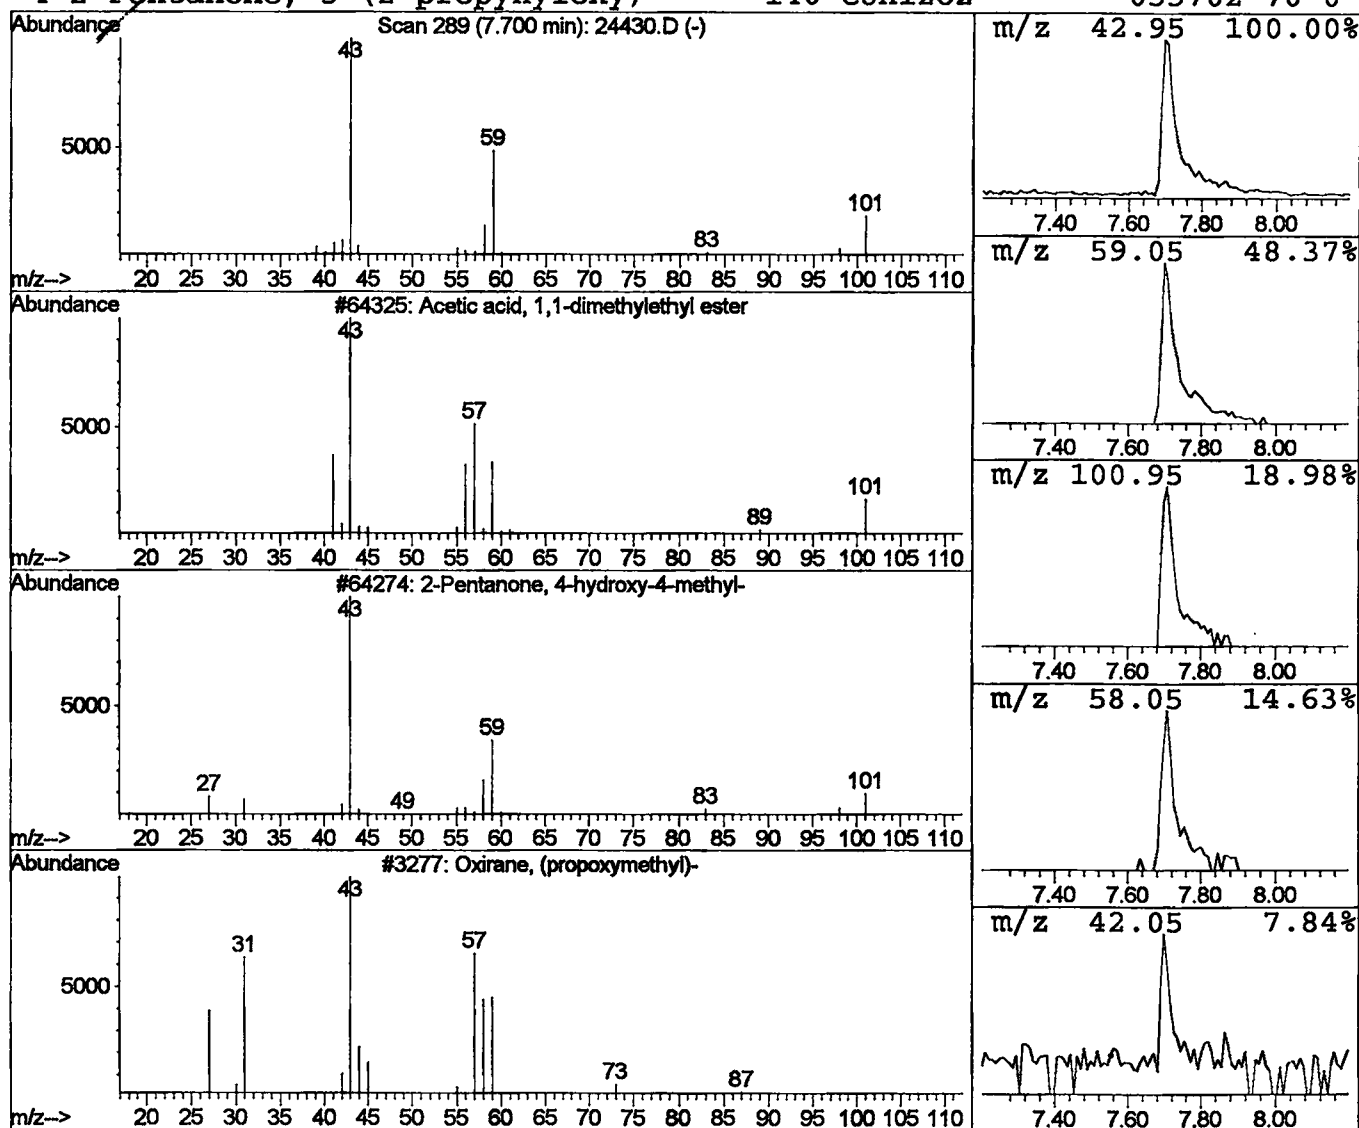

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\NOV0201\24430.D
Acq On : 2 Nov 2001 9:52 pm
Sample : gc/ms unknown
Misc :
MS Integration Params: LSCINT.P


Vial: 8
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 2 1,4-Dichlorobenzene-d4 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.57	0.53 ug/l	76511	1,4-Dichlorobenzene-d4	11.71

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1,4-Dichlorobenzene-d4	150	C6Cl2D4	003855-82-1	50
2			Benzene-1,2,3,4-d4-, 5,6-dichloro-	150	C6Cl2D4	002199-69-1	32
3			Benzenamine, 2-methyl-4-nitro-	152	C7H8N2O2	000099-52-5	22
4			Benzenamine, 2-methyl-5-nitro-	152	C7H8N2O2	000099-55-8	14

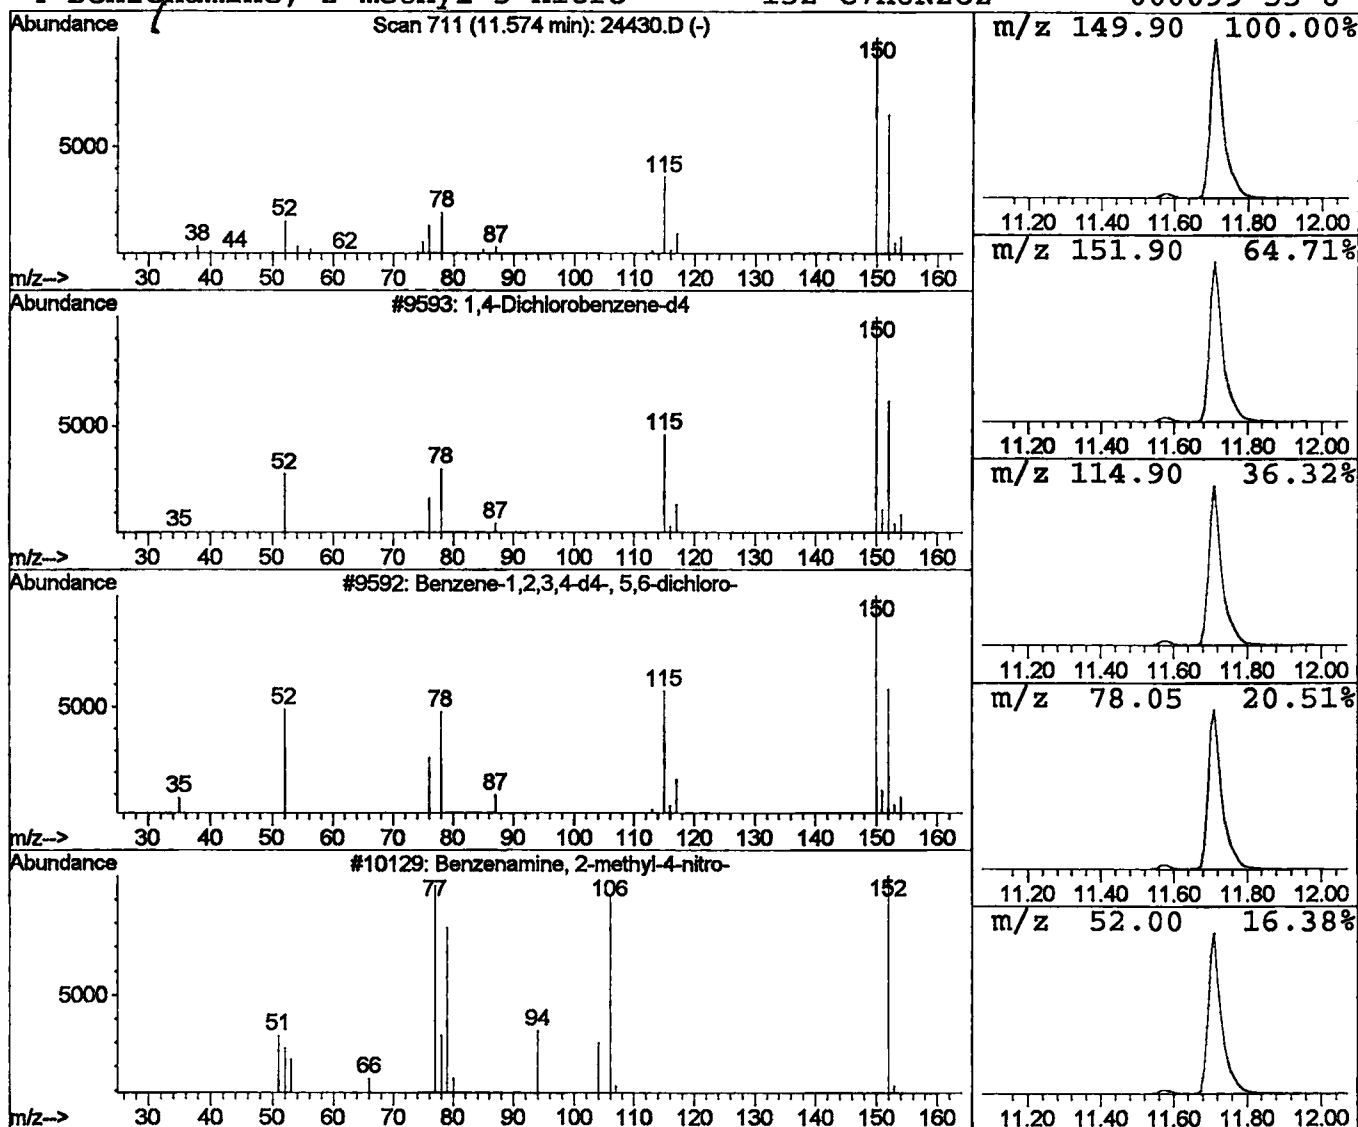

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 2 Nov 2001 9:52 pm
Data File: C:\HPCHEM\1\DATA\NOV0201\24430.D
Name: gc/ms unknown
Misc:
Method: C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
Acetic acid, 1,1-dim	7.70	0.5	ug/l	73456	ISTD01	11.71	2909540	20.0
1,4-Dichlorobenzene-	11.57	0.5	ug/l	76511	ISTD01	11.71	2909540	20.0

24430.D NP103001.M Tue Nov 06 08:06:59 2001