

Method 508 GCMS Date Extracted 10/12/01Page 28

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH =7	Count		
	labile	500ul		1ml	-	-	2ml					
	Reference Pest											
	MDL Pest											
	PRL 1260											
	24421 ✓									9		
	24422 ✓									10		
	24473 ✓									11		
	24474 ✓									12		
	24475 ✓									13		
	24476 ✓									14		
	24477 ✓									15		
	24478 ✓									16		
	24479 ✓									17		
	24480 ✓									18		
	24481 ✓									19		
	23344 500ul											
	23354											
Remarks												
23344 > re extracted												
23354 for GC/MS												
Reviewed by <u>DN</u> 11/14/01												
drip rate must be between 5-15 ml/min for liq-liq extractors												
Extraction type <u>Syphum</u> Solv. lot# <u>NaCl lot# 12617</u> Na2SO4 lot# <u>8024 V32603</u>												
STANDARD	INT STD LOG#											
CALIBRATION												
REF/SPIKE	<u>Prot 20604</u>	<u>PRL 1260</u>										
MDL/MDRF												
Q. CHECK												
INT. STD.												
SURROGATE	<u>20646</u>											
LPC												
ENDRIN/DDT												

Analyst my/cm/AD
revision 4/12/01

Verified by _____

Reviewed by DN
Date 11/14/01

Sequence Name: C:\HPCHEM\1\SEQUENCE\NOV0201.S

Comment: INST 209; 30Mx0.25umX0.50

Operator: 209 GALOS

Data Path: C:\HPCHEM\1\data\nov0201\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run

On A Barcode Mismatch

☒ Full Method☒ Inject Anyway☐ Reprocessing Only☐ Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	NP103001	
2	Sample	2	24429	NP103001	gc/ms unknown
3	Sample	3	24397	NP103001	gc/ms unknown
4	Sample	4	24398	NP103001	gc/ms unknown
5	Sample	5	24399	NP103001	gc/ms unknown
6	Sample	6	24400	NP103001	gc/ms unknown
7	Sample	7	24401	NP103001	gc/ms unknown
8	Sample	8	24430	NP103001	gc/ms unknown
9	Sample	9	LB	NP103001	10/12
10	Sample	10	23344	NP103001	gc/ms unknown reextract
11	Sample	11	24431	NP103001	gc/ms unknown
12	Sample	12	24476	NP103001	gc/ms unknown
13	Sample	13	24477	NP103001	gc/ms unknown
14	Sample	14	24474	NP103001	gc/ms unknown
15	Sample	15	24479	NP103001	gc/ms unknown
16	Sample	16	24478	NP103001	gc/ms unknown
17	Sample	17	24473	NP103001	gc/ms unknown
18	Sample	18	24480	NP103001	gc/ms unknown
19	Sample	19	24475	NP103001	gc/ms unknown
20	Sample	20	24481	NP103001	gc/ms unknown
21	Sample	21	24482	NP103001	gc/ms unknown
22	Sample	22	24483	NP103001	gc/ms unknown
23	Sample	23	24484	NP103001	gc/ms unknown
24	Sample	24	24485	NP103001	gc/ms unknown
25	Sample	25	24486	NP103001	gc/ms unknown

24472 analysis
done on 10/14

DFTPP

Data File : C:\HPCHEM\1\DATA\NOV0201\DFTPP.D

Acq On : 2 Nov 2001 2:58 pm

Sample :

Misc :

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

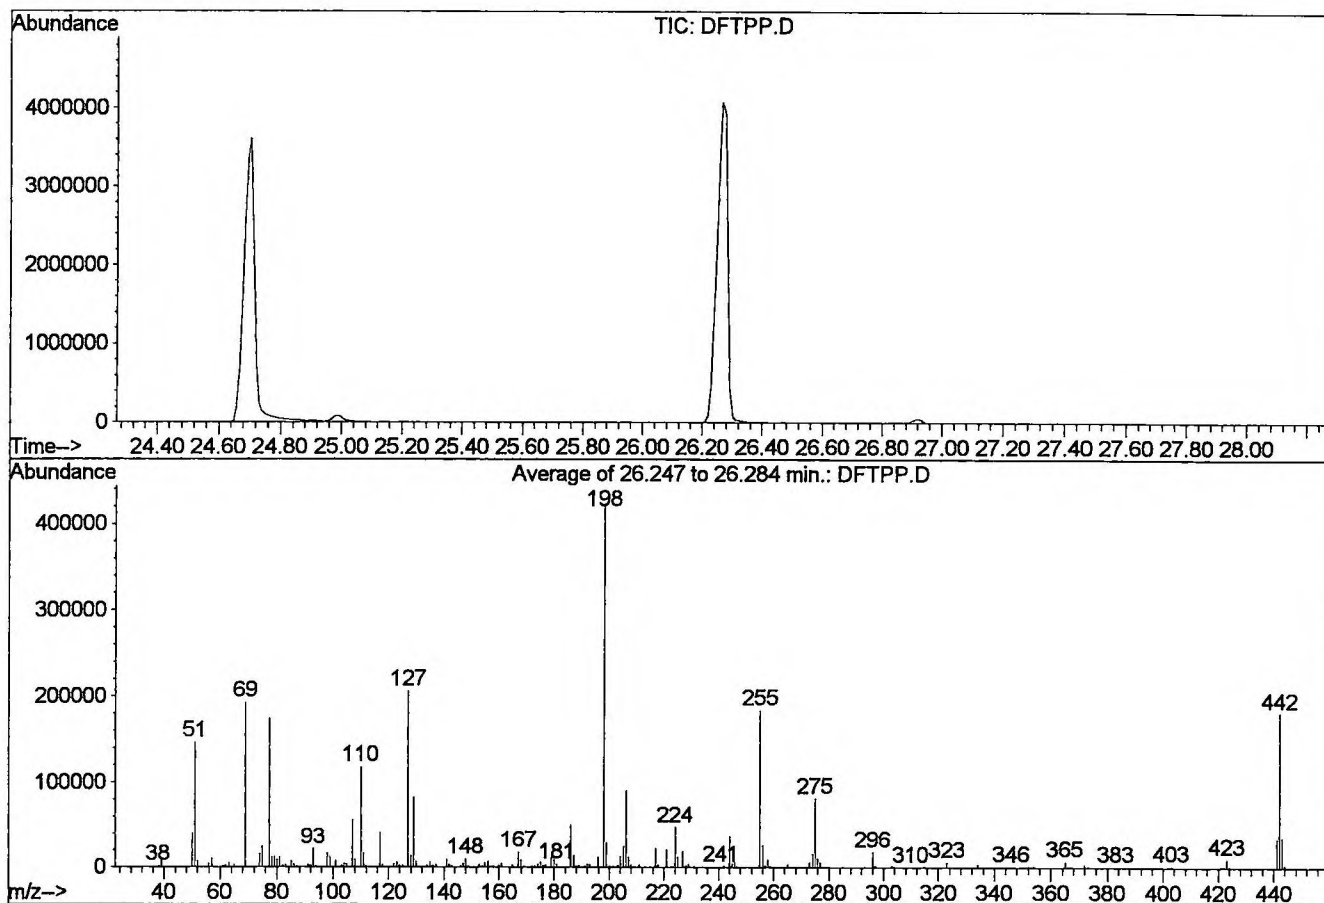

Spectrum Information: Average of 26.247 to 26.284 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	34.6	146181	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	45.5	192600	PASS
70	69	0.00	2	0.1	177	PASS
127	198	40	60	48.8	206254	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	422861	PASS
199	198	5	9	6.8	28922	PASS
275	198	10	30	19.4	82128	PASS
365	198	1	100	1.6	6942	PASS
441	443	0.01	100	96.2	33651	PASS
442	198	40	110	42.7	180502	PASS
443	442	17	23	19.4	34984	PASS

DFTPP.D NP103001.M

Fri Nov 02 15:51:43 2001