

Method

SOS SCSMS
Seen

Date Extracted

10/16/01

Page

33

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
	lab blank	SPONGE	✓	1ml		-	2ml		7			
	Reference Chloride											
	MDL Chlor											
	PRC1221											
24487	spike post				1ml							
24487	spike dup post											
24488	spike TOX											
24488	spike dup TOX											
24487	✓								3	12		
24488	✓									13		
24489	✓									14		
24490	✓									15		
24491	✓									16		
24492	✓									17		
24493	✓									18		
24640	✓									19		
24641	✓									20		
24642	✓									1		
24644	✓									2		
24645	✓									3		
Reviewed by, 10/22/02												
Remarks												
drip rate must be between 5-15 ml/min for liq-liq extractors												
Extraction type - <u>Sephenel</u> Solv.lot# <u>NaCl lot# T12417</u> Na2SO4 lot# <u>8064 832600</u>												
STANDARD	INT STD LOG#											
CALIBRATION												
REF/SPIKE	chlor. 1780	post 2064	1678				PRC1221 - 1501					
MDL/MDRF												
Q. CHECK												
INT. STD.												
SURROGATE	2064											
LPC												
ENDRIN/DDT												

Analyst CM/AM
revision 4/12/01

Verified by _____

Reviewed by AM
Date 11/21/01

Sequence Name: C:\HPCHEM\1\SEQUENCE\NOV0501.S
 Comment: INST 209; 30Mx0.25umX0.50
 Operator: 209 GALOS
 Data Path: C:\HPCHEM\1\data\nov0501\
 Pre-Seq Cmd:
 Post-Seq Cmd:


Method Sections To Run On A Barcode Mismatch
☒ Full Method ☒ Inject Anyway
☐ Reprocessing Only ☐ Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	NP103001	
2	Sample	1	DFTPP1	NP103001	
3	Sample	2	LB	NP103001	10/16 lab blk
4	Sample	3	24493	NP103001	gc/ms unknown
5	Sample	4	24695	NP103001	gc/ms unknown
6	Sample	5	24487	NP103001	gc/ms unknown
7	Sample	6	24488	NP103001	gc/ms unknown
8	Sample	7	24694	NP103001	gc/ms unknown
9	Sample	8	24492	NP103001	gc/ms unknown
10	Sample	9	24642	NP103001	gc/ms unknown
11	Sample	10	24491	NP103001	gc/ms unknown
12	Sample	11	24641	NP103001	gc/ms unknown
13	Sample	12	24489	NP103001	gc/ms unknown
14	Sample	13	24640	NP103001	gc/ms unknown
15	Sample	14	24490	NP103001	gc/ms unknown
16	Sample	15	LBA	NP103001	10/17 lb
17	Sample	16	24697	NP103001	gc/ms unknown
18	Sample	17	24696	NP103001	gc/ms unknown
19	Sample	18	24699	NP103001	gc/ms unknown
20	Sample	19	24698	NP103001	gc/ms unknown
21	Sample	20	24730	NP103001	gc/ms unknown
22	Sample	21	24700	NP103001	gc/ms unknown
23	Sample	1	DFTPP2	NP103001	
24	Sample	22	24879	NP103001	gc/ms unknown
25	Sample	23	24874	NP103001	gc/ms unknown
26	Sample	24	24878	NP103001	gc/ms unknown

DFTPP

Data File : C:\HPCHEM\1\data\nov0501\DFTPP1.D
 Acq On : 5 Nov 2001 11:16 am
 Sample :
 Misc :
 MS Integration Params: RTEINT.P
 Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

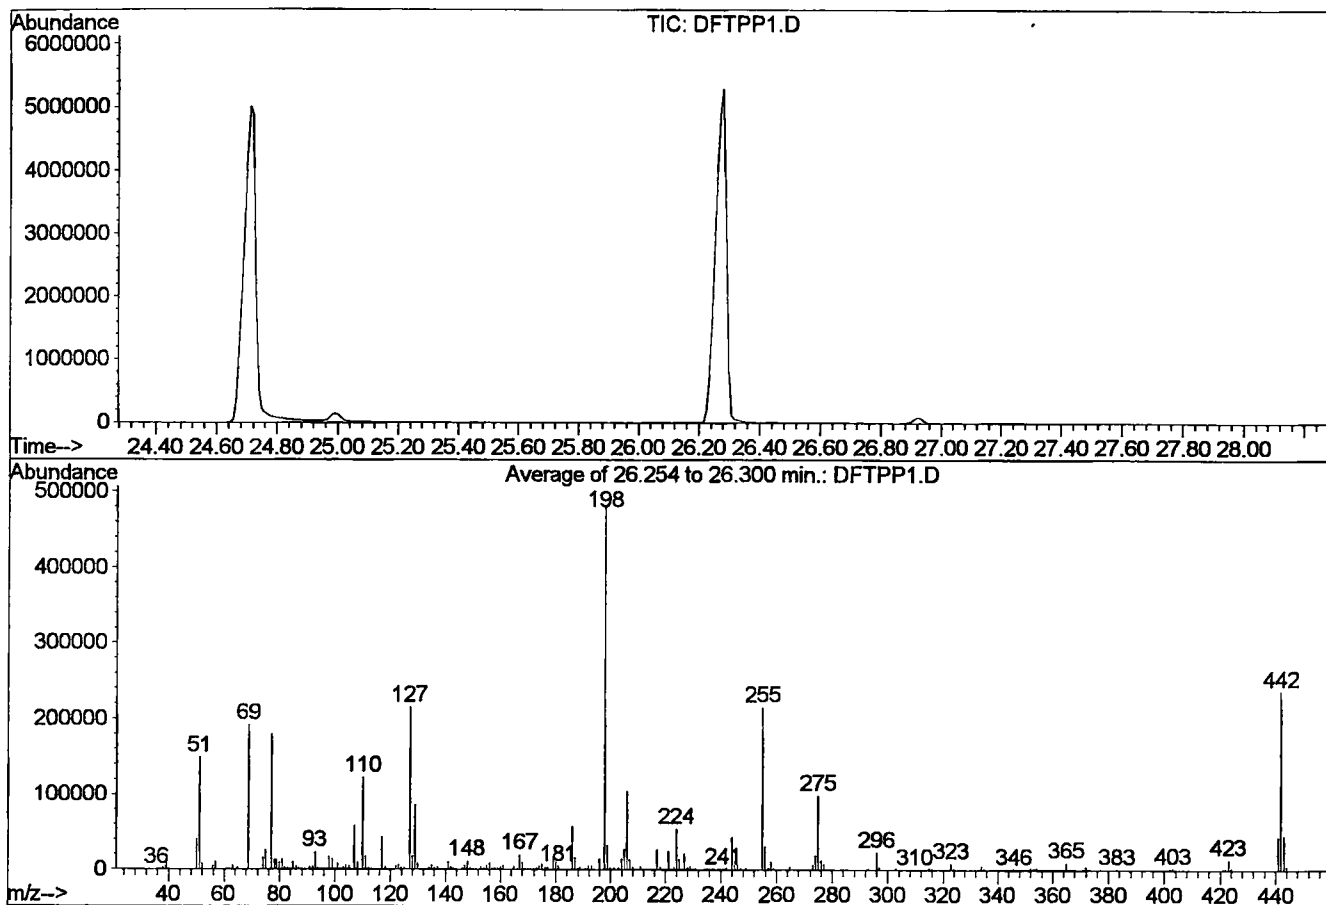

Spectrum Information: Average of 26.254 to 26.300 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	30.9 ✓	148929	PASS
68	69	0.00	2	0.0 ✓	0	PASS
69	198	0.00	100	39.9 ✓	192137	PASS
70	69	0.00	2	0.0 ✓	33	PASS
127	198	40	60	44.8 ✓	215811	PASS
197	198	0.00	1	0.0 ✓	0	PASS
198	198	100	100	100.0 ✓	481809	PASS
199	198	5	9	6.7 ✓	32083	PASS
275	198	10	30	20.5 ✓	98865	PASS
365	198	1	100	2.0 ✓	9479	PASS
441	443	0.01	100	95.8 ✓	43059	PASS
442	198	40	110	49.1 ✓	236725	PASS
443	442	17	23	19.0	44957	PASS

DFTPP1.D NP103001.M 5 Mon Nov 05 11:52:19 2001