

Method 508Date Extracted 10/15/01Page 31QCM8

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count
	Lab 1016	500ml	—	1ml		—	2ml		7	
	Reference Triphenyl									
	MDL TOX									
	PRC 1016									
	Spike past			1ml						
	Spike past									
	Spike Chloroform									
	Spike Chloro									
	24482									20
	24483									1
	24484									2
	24485									3
	24486									4
	23342									5
	23341									6
	23345									7
	23340									8
	23472									9
	23359									10
	23344									11
	24333									
Reviewed by <u>2/13/02</u>										
Remarks										
drip rate must be between 5-15 ml/min for liq-liq extractors										
drip rate -										
Extraction type <u>Sephadex</u> Solv. lot# <u>T12417</u> NaCl lot# <u>8024 V32603</u>										
STANDARD	INT STD LOG#									
CALIBRATION										
REF/SPIKE										
MDL/MDRF										
Q. CHECK										
INT. STD.										
SURROGATE										
LPC										
ENDRIN/DDT										

Analyst My/AD/CM
revision 4/12/01

Verified by _____

Reviewed by DP
Date 11/13/01

Sequence Name: C:\HPCHEM\1\SEQUENCE\NOV0201.S
 Comment: INST 209; 30Mx0.25umX0.50
 Operator: 209 GALOS
 Data Path: C:\HPCHEM\1\data\nov0201\
 Pre-Seq Cmd:
 Post-Seq Cmd:

Method Sections To Run On A Barcode Mismatch
☒ (X) Full Method ☒ (X) Inject Anyway
☐ () Reprocessing Only ☐ () Don't Inject

Line Type	Vial	DataFile	Method	Sample Name
1 Sample	1	DFTPP	NP103001	
2 Sample	2	24429	NP103001	gc/ms unknown
3 Sample	3	24397	NP103001	gc/ms unknown
4 Sample	4	24398	NP103001	gc/ms unknown
5 Sample	5	24399	NP103001	gc/ms unknown
6 Sample	6	24400	NP103001	gc/ms unknown
7 Sample	7	24401	NP103001	gc/ms unknown
8 Sample	8	24430	NP103001	gc/ms unknown
9 Sample	9	LB	NP103001	10/12
10 Sample	10	23344	NP103001	gc/ms unknown reextract
11 Sample	11	24431	NP103001	gc/ms unknown
12 Sample	12	24476	NP103001	gc/ms unknown
13 Sample	13	24477	NP103001	gc/ms unknown
14 Sample	14	24474	NP103001	gc/ms unknown
15 Sample	15	24479	NP103001	gc/ms unknown
16 Sample	16	24478	NP103001	gc/ms unknown
17 Sample	17	24473	NP103001	gc/ms unknown
18 Sample	18	24480	NP103001	gc/ms unknown
19 Sample	19	24475	NP103001	gc/ms unknown
20 Sample	20	24481	NP103001	gc/ms unknown
21 Sample	21	24482	NP103001	gc/ms unknown
22 Sample	22	24483	NP103001	gc/ms unknown
23 Sample	23	24484	NP103001	gc/ms unknown
24 Sample	24	24485	NP103001	gc/ms unknown
25 Sample	25	24486	NP103001	gc/ms unknown

DFTPP

Data File : C:\HPCHEM\1\DATA\NOV0201\DFTPP.D

Acq On : 2 Nov 2001 2:58 pm

Sample :

Misc :

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

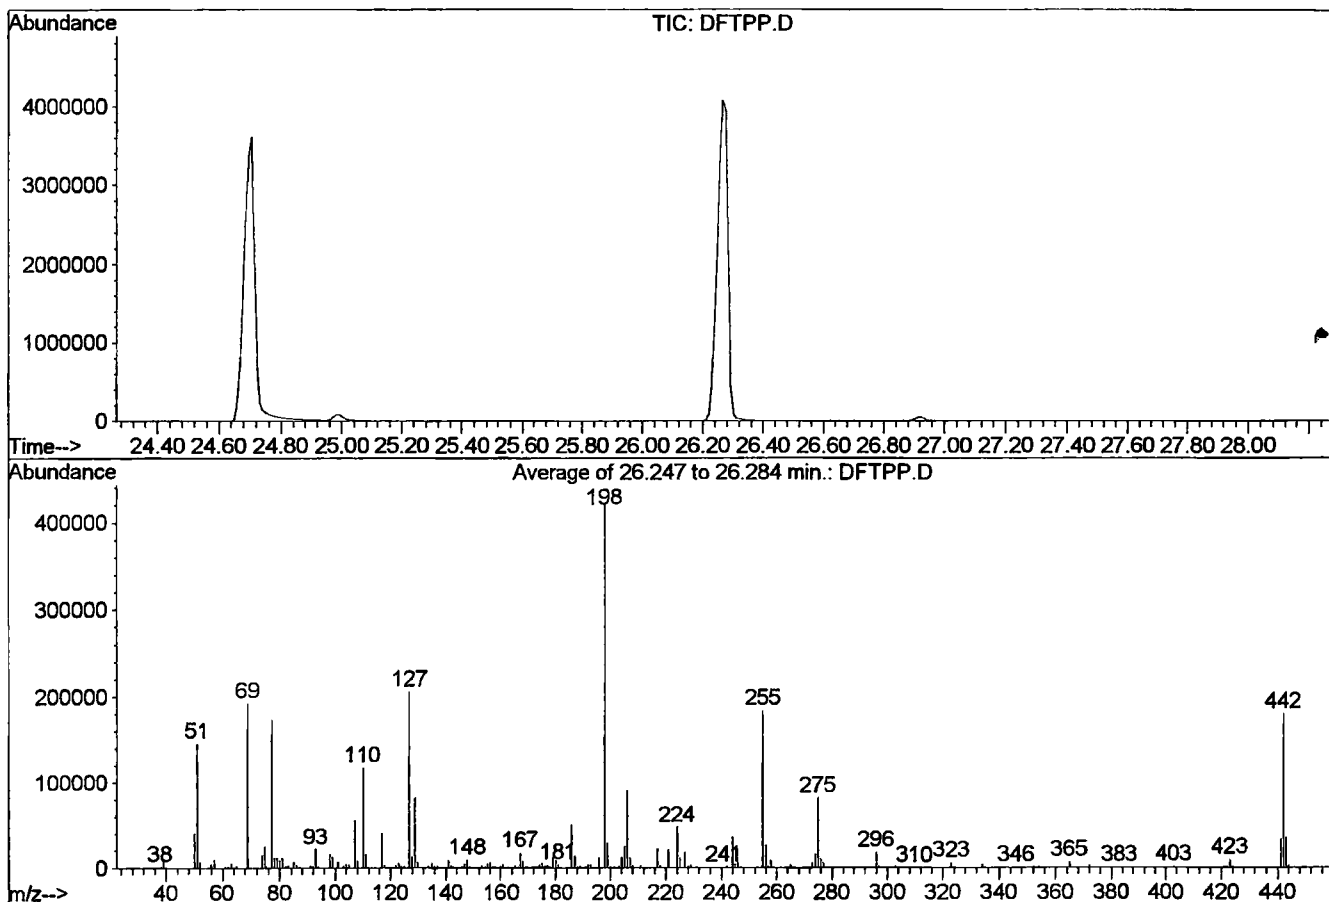

Spectrum Information: Average of 26.247 to 26.284 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	34.6 ✓	146181	PASS
68	69	0.00	2	0.0 ✓	0	PASS
69	198	0.00	100	45.5 ✓	192600	PASS
70	69	0.00	2	0.1 ✓	177	PASS
127	198	40	60	48.8 ✓	206254	PASS
197	198	0.00	1	0.0 ✓	0	PASS
198	198	100	100	100.0 ✓	422861	PASS
199	198	5	9	6.8 ✓	28922	PASS
275	198	10	30 ✓	19.4 ✓	82128	PASS
365	198	1	100	1.6 ✓	6942	PASS
441	443	0.01	100	96.2 ✓	33651	PASS
442	198	40	110	42.7 ✓	180502	PASS
443	442	17	23	19.4 ✓	34984	PASS

DFTPP.D NP103001.M

Tue Nov 13 11:37:05 2001