

Method 508 GCMS
ScanDate Extracted 10/17/01Page 34

Lab #	Description	Sample	Drip rate	Surr	Spk	IS	Final	T.V.	pH	Count		
		vol/wt	ml/min	add	add	add	vol.	pos.	=7			
	6064h	500ul	—	1ul	—	—	2ul					
	Reference peak											
	MDL peak											
✓	PRL 1232											
✓	24696									4		
✓	24697									5		
✓	24698									6		
✓	24699									7		
✓	24700									8		
✓	24730									9		
✓	24731									10		
✓	24732									11		
	24816									12		
	24822									13		
	24824									14		
✓	24872									15		
✓	24873									16		
✓	24874									17		
✓	24875									18		
✓	24876									19		
✓	24877									20		
✓	24878											
✓	24879											
Remarks												
Reviewed by <u>[Signature]</u> 11/20/01												
drip rate must be between 5-15 ml/min for liq-liq extractors			drip rate -									
Extraction type -		Solv.lot#		NaCl lot#		12617		Na2SO4 lot#		8064 V 32603		
STANDARD	INT STD LOG#											
CALIBRATION												
REF/SPIKE	peak 2062a											
MDL/MDRF	PRL 1232 1502											
Q. CHECK												
INT. STD.												
SURROGATE	2064c											
LPC												
ENDRIN/DDT												

Analyst ADJCM
revision 4/12/01

Verified by _____

Reviewed by [Signature]
Date 11/20/01

Sequence Name: C:\HPCHEM\1\SEQUENCE\NOV0601.S

Comment: INST 209; 30Mx0.25umX0.50

Operator: 209 GALOS

Data Path: C:\HPCHEM\1\data\nov0601\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run	On A Barcode Mismatch
(X) Full Method	(X) Inject Anyway
() Reprocessing Only	() Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	24293	NP103001	gc/ms unknown
2	Sample	2	24873✓	NP103001	gc/ms unknown
3	Sample	3	24872✓	NP103001	gc/ms unknown
4	Sample	4	24877✓	NP103001	gc/ms unknown
5	Sample	5	24876✓	NP103001	gc/ms unknown
6	Sample	6	24732✓	NP103001	gc/ms unknown
7	Sample	7	24731✓	NP103001	gc/ms unknown
8	Sample	8	24875✓	NP103001	gc/ms unknown
9	Sample	9	LBA	NP103001	lb 10/18
10	Sample	10	24880	NP103001	gc/ms unknown
11	Sample	11	24944	NP103001	gc/ms unknown
12	Sample	12	24881	NP103001	gc/ms unknown
13	Sample	13	24945	NP103001	gc/ms unknown
14	Sample	14	24946	NP103001	gc/ms unknown
15	Sample	15	24947	NP103001	gc/ms unknown
16	Sample	16	24948	NP103001	gc/ms unknown
17	Sample	17	24949	NP103001	gc/ms unknown
18	Sample	18	24950	NP103001	gc/ms unknown
19	Sample	19	24982	NP103001	gc/ms unknown

DFTPP

Data File : C:\HPCHEM\1\DATA\NOV0501\DFTPP2.D

Acq On : 6 Nov 2001 8:26 am

Sample :

Misc :

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

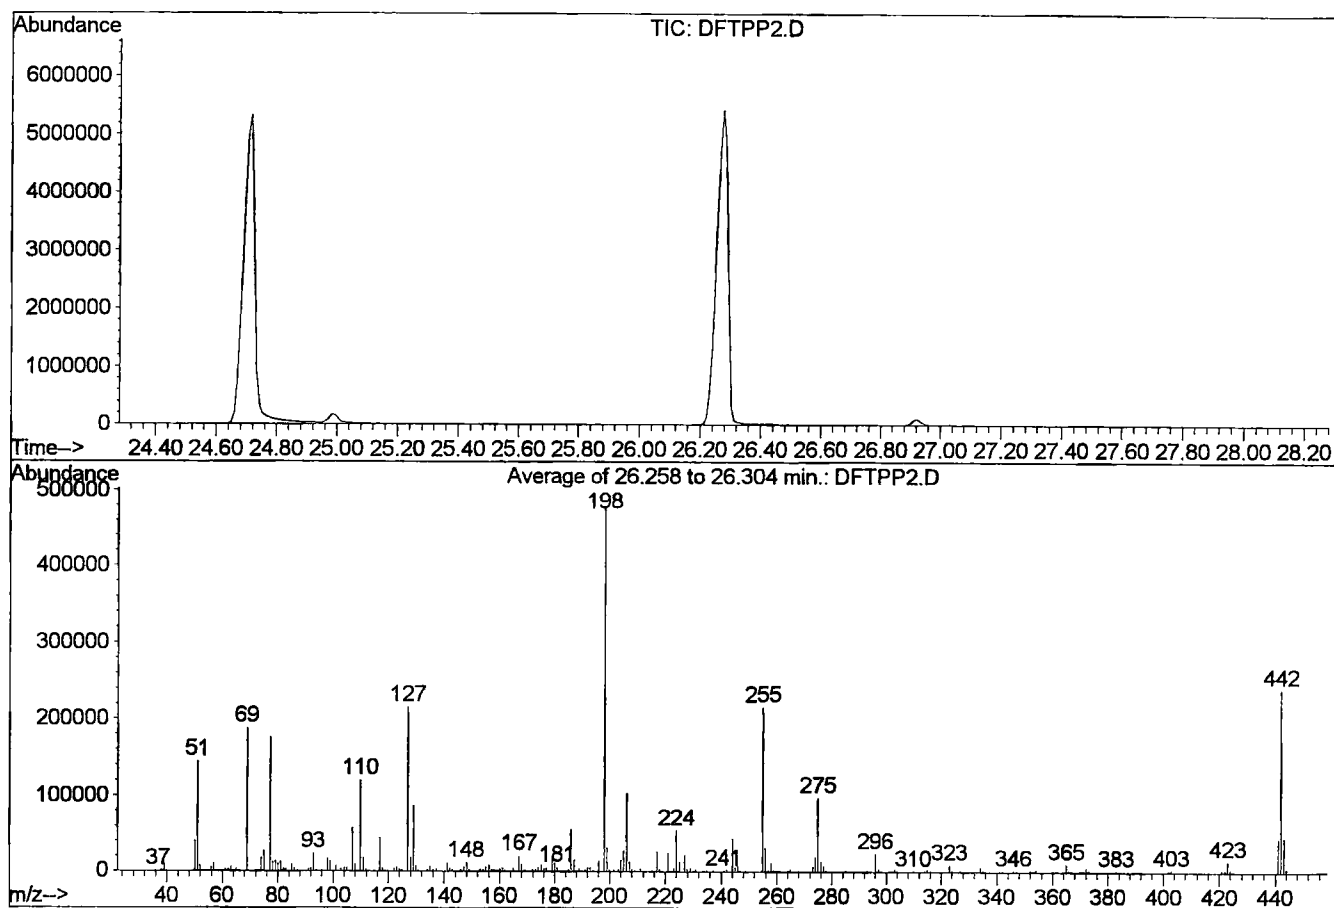

Spectrum Information: Average of 26.258 to 26.304 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	30.3	144707	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	39.3	187808	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	45.0	215484	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	478339	PASS
199	198	5	9	6.6	31722	PASS
275	198	10	30	20.5	97823	PASS
365	198	1	100	2.0	9641	PASS
441	443	0.01	100	95.9	43427	PASS
442	198	40	110	49.9	238721	PASS
443	442	17	23	19.0	45272	PASS

DFTPP2.D NP103001.M

Tue Nov 06 11:25:18 2001