

User: Galos, Marie
 Westchester Dept. of Labs & Research
 Date: 11/19/2001 Time: 09:53:05

Sample: AD24880
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 11/19/01 09:49 Ended: 11/19/01 09:49 Analyst: MG
 Page: 1

Component Name	Viol	Result
Other unknown compounds		see comment

Comments for Sample AD24880 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Galos, Marie

Date: 11-19-2001 Time: 09:53:10

A scan of the extract prepared for the 508 analysis, from 35-550 amu using a mass spectrometer, does not reveal the presence of non-target compounds.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV0601\24880.D
 Acq On : 6 Nov 2001 9:34 pm
 Sample : gc/ms unknown
 Misc :
 MS Integration Params: RTEINT.P
 Quant Time: Nov 6 22:23 2001

Vial: 10
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: NP103001.RES

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Fri Nov 02 16:41:16 2001
 Response via : Initial Calibration
 DataAcq Meth : NP103001

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	11.72	152	668925	20.00	ug/l	0.00
19) Naphthalene-d8	15.32	136	2547276	20.00	ug/l	0.00
31) Acenaphthene-d10	20.59	164	1259888	20.00	ug/l	-0.02
49) Phenanthrene-d10	25.02	188	1912702	20.00	ug/l	-0.02
59) Chrysene-d12	33.06	240	1379257	20.00	ug/l	0.00
68) Perylene-d12	37.16	264	1009319	20.00	ug/l	0.00

System Monitoring Compounds

4) 2-Fluorophenol	0.00	112	0	0.00	ug/l	
Spiked Amount	75.000		Recovery	=	0.00%	
5) Phenol-d5	0.00	99	0	0.00	ug/l	
Spiked Amount	75.000		Recovery	=	0.00%	
6) 2-Chlorophenol-d4	0.00	132	0	0.00	ug/l	
Spiked Amount	75.000		Recovery	=	0.00%	
7) 1,2-Dichlorobenzene-d4	12.24	152	7780	0.26	ug/l	0.00
Spiked Amount	50.000		Recovery	=	0.52%	
20) Nitrobenzene-d5	0.00	82	0	0.00	ug/l	
Spiked Amount	50.000		Recovery	=	0.00%	
32) 2-Fluorobiphenyl	18.75	172	2637	0.03	ug/l	0.13
Spiked Amount	50.000		Recovery	=	0.06%	
33) 2,4,6-Tribromophenol	0.00	330	0	0.00	ug/l	
Spiked Amount	75.000		Recovery	=	0.00%	
62) Terphenyl-d14	0.00	244	0	0.00	ug/l	
Spiked Amount	50.000		Recovery	=	0.00%	

Target Compounds

					Qvalue
2) Pyridine	0.00	79	0	N.D.	
3) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
8) Phenol	0.00	94	0	N.D.	
9) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
10) 2-Chlorophenol	0.00	128	0	N.D.	
11) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
12) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
13) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
14) 2-Methylphenol	0.00	108	0	N.D.	
15) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
16) 3&4-Methylphenol	0.00	108	0	N.D.	
17) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
18) Hexachloroethane	0.00	117	0	N.D.	
21) Nitrobenzene	0.00	77	0	N.D.	
22) Isophorone	0.00	82	0	N.D.	

(#) = qualifier out of range (m) = manual integration

24880.D NP103001.M Fri Nov 16 12:04:56 2001

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV0601\24880.D

Vial: 10

Acq On : 6 Nov 2001 9:34 pm

Operator: 209 GALOS

Sample : gc/ms unknown

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Nov 6 22:23 2001

Quant Results File: NP103001.RES

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Nov 02 16:41:16 2001

Response via : Initial Calibration

DataAcq Meth : NP103001

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
23) 2-Nitrophenol	0.00	139	0	N.D.		
24) 2,4-Dimethylphenol	0.00	107	0	N.D.		
25) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.		
26) 2,4-Dichlorophenol	0.00	162	0	N.D.		
27) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.		
28) Naphthalene	15.37	128	527	N.D.		
29) Hexachlorobutadiene	0.00	225	0	N.D.		
30) 4-Chloro-3-methylphenol	0.00	107	0	N.D.		
34) Hexachlorocyclopentadiene	0.00	237	0	N.D.		
35) 2,4,6-Trichlorophenol	0.00	196	0	N.D.		
36) 2,4,5-Trichlorophenol	0.00	196	0	N.D.		
37) 2-Chloronaphthalene	0.00	162	0	N.D.		
38) Dimethylphthalate	0.00	163	0	N.D.		
39) 2,6-Dinitrotoluene	0.00	165	0	N.D.		
40) Acenaphthylene	0.00	152	0	N.D.		
41) Acenaphthene	0.00	153	0	N.D.		
42) 2,4-Dinitrophenol	0.00	184	0	N.D.		
43) 4-Nitrophenol	0.00	65	0	N.D.		
44) 2,4-Dinitrotoluene	21.03	165	185	N.D.		
45) Diethylphthalate	0.00	149	0	N.D.		
46) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.		
47) Fluorene	0.00	166	0	N.D.		
48) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.		
50) 4,6-Dinitro-2-methylphenol	0.00	198	0	N.D.		
51) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
52) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
53) Hexachlorobenzene	0.00	284	0	N.D.		
54) Pentachlorophenol	0.00	266	0	N.D.		
55) Phenanthrene	25.03	178	374	N.D.		
56) Anthracene	25.03	178	374	N.D.		
57) Di-n-butylphthalate	27.04	149	3661	N.D.		
58) Fluoranthene	0.00	202	0	N.D.		
60) 3,3'-Dichlorobenzidine	0.00	252	0	N.D.		
61) Benzidine	0.00	184	0	N.D.		
63) Pyrene	0.00	202	0	N.D.		
64) Butylbenzylphthalate	0.00	149	0	N.D.		
65) Benzo(a)anthracene	33.06	228	3526	N.D.		
66) Bis(2-ethylhexyl)phthalate	33.34	149	1186	N.D.		
67) Chrysene	33.06	228	3526	N.D.		
69) Di-n-Octylphthalate	0.00	149	0	N.D.		
70) Benzo(b)fluoranthene	0.00	252	0	N.D.		

(#)=qualifier out of range (m)=manual integration

24880.D NP103001.M Fri Nov 16 12:04:59 2001

Page 2

Quantitation Report (QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV0601\24880.D

Vial: 10

Acq On : 6 Nov 2001 9:34 pm

Operator: 209 GALOS

Sample : gc/ms unknown

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Nov 6 22:23 2001

Quant Results File: NP103001.RES

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Nov 02 16:41:16 2001

Response via : Initial Calibration

DataAcq Meth : NP103001

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
71) Benzo(k)fluoranthene	0.00	252	0	N.D.		
72) Benzo(a)pyrene	37.16	252	3864	N.D.		
73) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
74) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
75) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

24880.D NP103001.M Fri Nov 16 12:04:59 2001

Page 3


Quantitation Report

Data File : C:\HPCHEM\1\DATA\NOV0601\24880.D
Acq On : 6 Nov 2001 9:34 pm
Sample : gc/ms unknown
Misc :
MS Integration Params: RTEINT.P
Quant Time: Nov 6 22:23 2001

Vial: 10
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: NP103001.RES

Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Fri Nov 02 16:41:16 2001
Response via : Initial Calibration

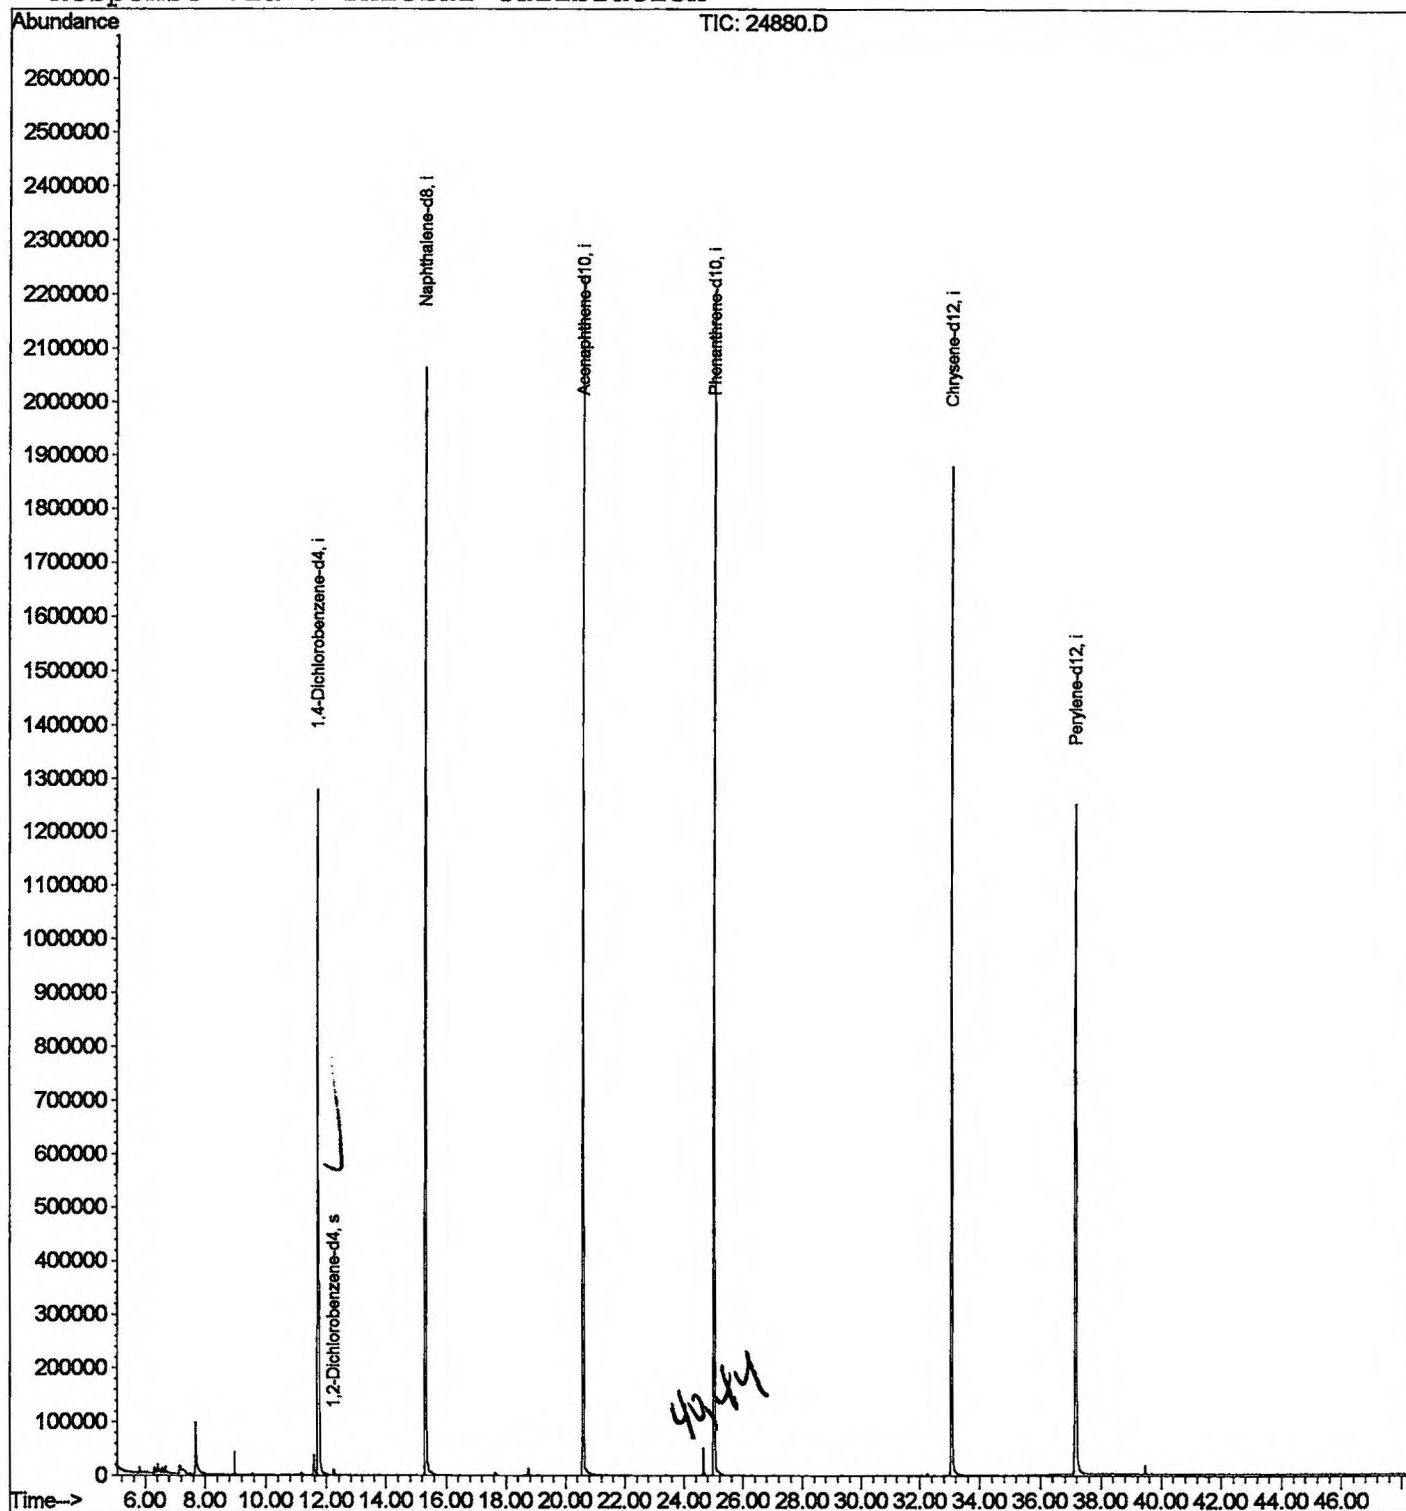

24880.D NP103001.M

Fri Nov 16 12:05:02 2001

Page 4

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\NOV0601\24880.D
 Acq On : 6 Nov 2001 9:34 pm
 Sample : gc/ms unknown
 Misc :
 MS Integration Params: LSCINT.P

Vial: 10
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC




peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	7.686	285	288	304	rBV	97248	273773	5.52%	1.046%
2	11.578	707	712	721	rBV	37782	93857	1.89%	0.359%
3	11.716	721	727	745	rBV	1277596	3431375	69.21%	13.115%
4	15.314	1114	1119	1137	rBV	2063063	4616354	93.11%	17.644%
5	20.593	1688	1694	1710	rBV	2234125	4958187	100.00%	18.951%
6	25.018	2170	2176	2190	rBV2	2204443	4799615	96.80%	18.345%
7	33.060	3045	3052	3072	rBV2	1877755	4344450	87.62%	16.605%
8	37.163	3490	3499	3518	rBV2	1247225	3645682	73.53%	13.934%

Sum of corrected areas: 26163293

24880.D NP103001.M Fri Nov 16 12:00:56 2001

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\NOV0601\24880.D
Operator : 209 GALOS
Acquired : 6 Nov 2001 9:34 pm using AcqMethod NP103001
Instrument : GC/MS 209
Sample Name: gc/ms unknown
Misc Info :
Vial Number: 10
Quant File :NP103001.RES (RTE Integrator)

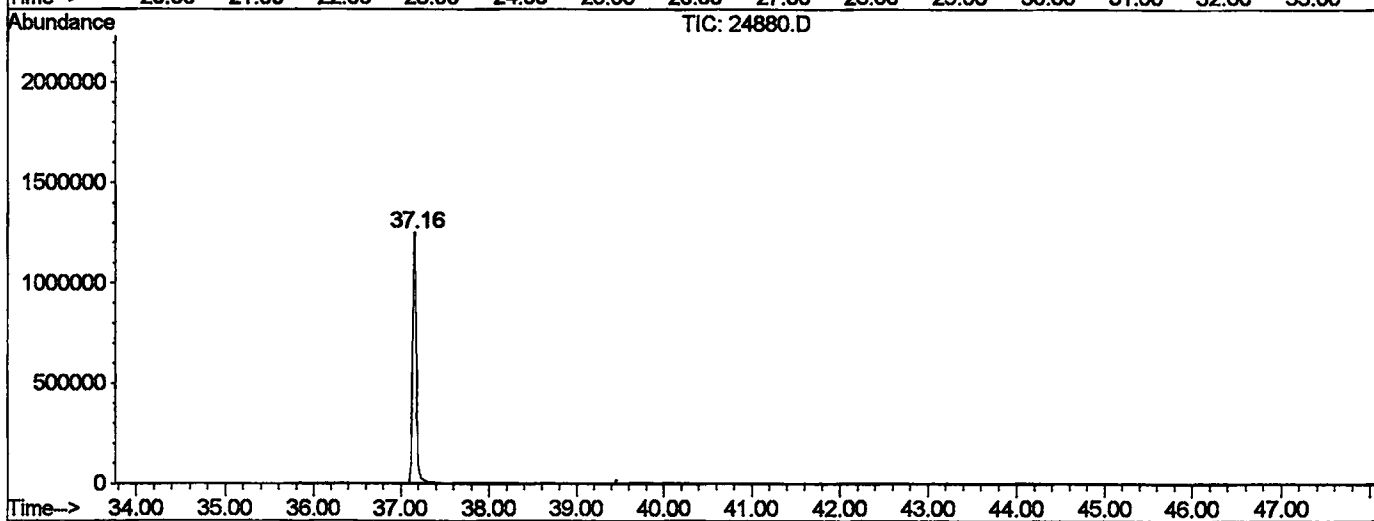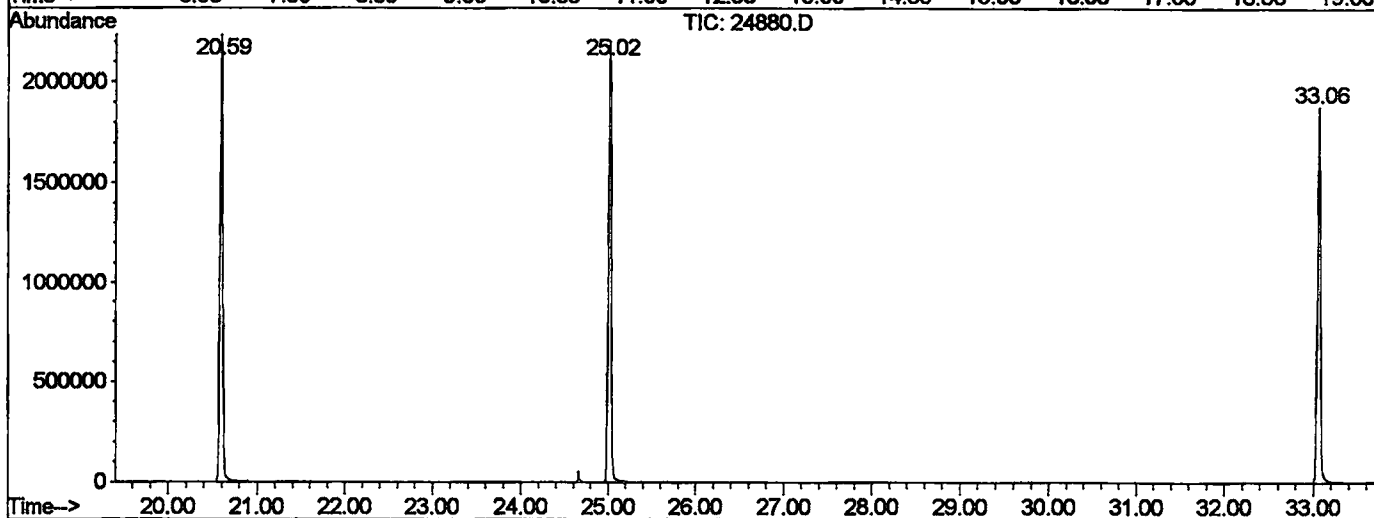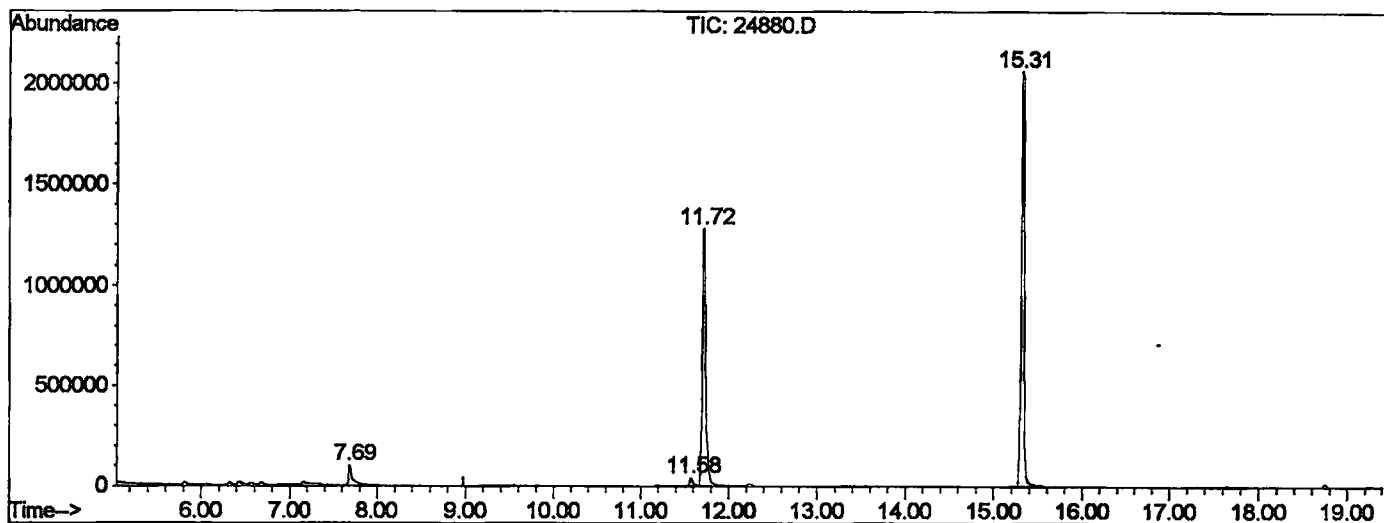

24880.D NP103001.M Fri Nov 16 12:00:58 2001

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\NOV0601\24880.D
 Acq On : 6 Nov 2001 9:34 pm
 Sample : gc/ms unknown
 Misc :
 MS Integration Params: LSCINT.P


Vial: 10
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.69	1.60 ug/l	273773	1,4-Dichlorobenzene-d4	11.72

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	40
2			2-Propanol, 2-methyl-	74	C4H10O	000075-65-0	17
3			Propanamide, n-ethyl-	101	C5H11NO	005129-72-6	9
4			Acetone	58	C3H6O	000067-64-1	9

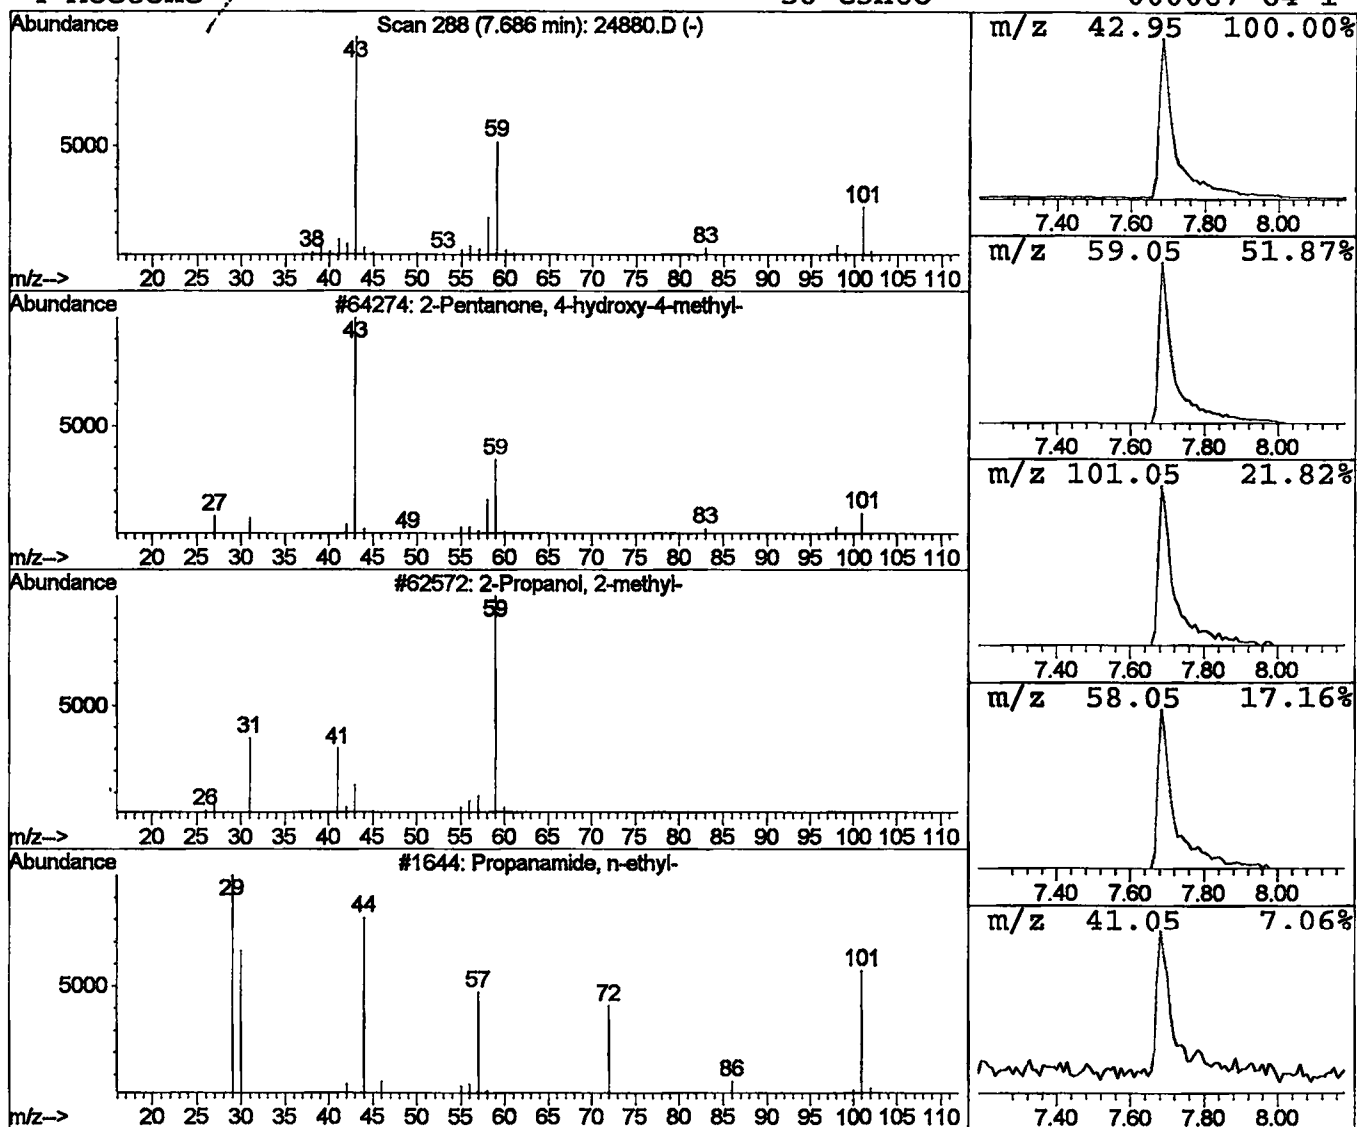

Library Search Compound Report


Data File : C:\HPCHEM\1\DATA\NOV0601\24880.D
Acq On : 6 Nov 2001 9:34 pm
Sample : gc/ms unknown
Misc :
MS Integration Params: LSCINT.P

Vial: 10
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 2 1,4-Dichlorobenzene-d4 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.	
11.58	0.55 ug/l	93857	1,4-Dichlorobenzene-d4	11.72	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	1,4-Dichlorobenzene-d4	150	C6Cl2D4	003855-82-1	90
2	Benzene-1,2,3,4-d4-, 5,6-dichloro-	150	C6Cl2D4	002199-69-1	33
3	2-Methyl-6-nitroaniline	152	C7H8N2O2	000570-24-1	10
4	3,4-Methylenedioxyanisole	152	C8H8O3	000000-00-0	9

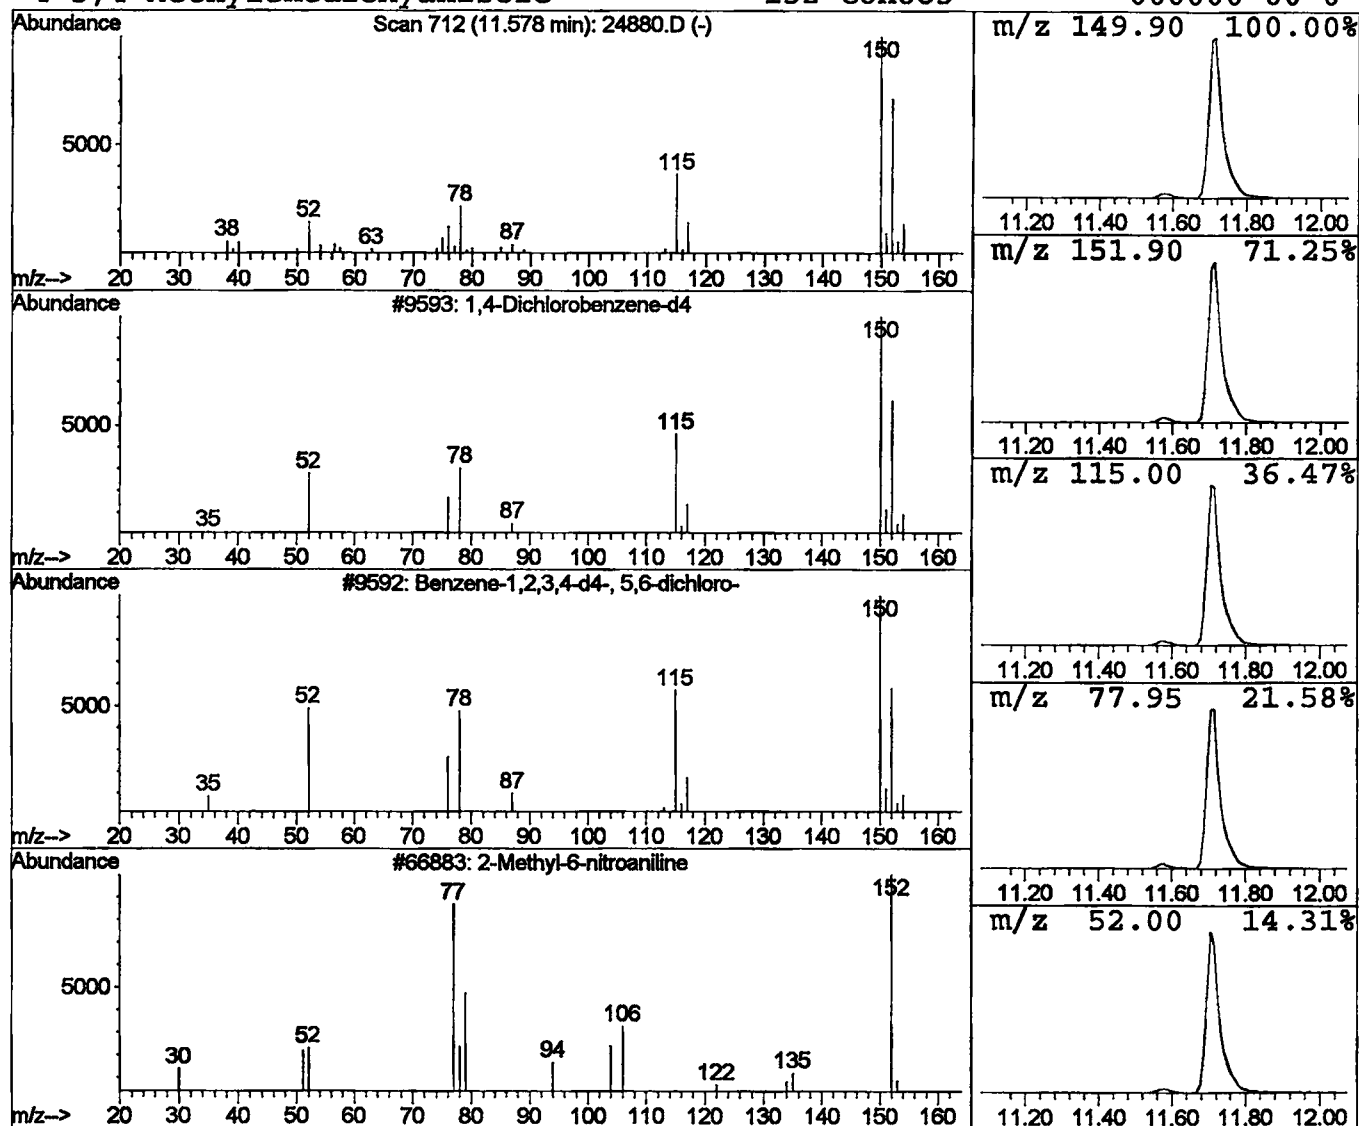

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 6 Nov 2001 9:34 pm
Data File: C:\HPCHEM\1\DATA\NOV0601\24880.D
Name: gc/ms unknown
Misc:
Method: C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	7.69	1.6	ug/l	273773	ISTD01	11.72	3431380	20.0
1,4-Dichlorobenzene-	11.58	0.5	ug/l	93857	ISTD01	11.72	3431380	20.0

24880.D NP103001.M Fri Nov 16 12:01:04 2001