

User: Galos, Marie
 Westchester Dept. of Labs & Research
 Date: 11/19/2001 Time: 09:53:51

Sample: AD24881
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 11/19/01 09:53 Ended: 11/19/01 09:53 Analyst: MG
 Page: 1

	Component Name	Vial	Result
1	Other unknown compounds		see comment

Comments for Sample AD24881 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Galos, Marie

Date: 11-19-2001 Time: 09:53:55

A scan of the extract prepared for the 508 analysis, from 35-550 amu using a mass spectrometer, does not reveal the presence of non-target compounds.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV0601\24881.D

Acq On : 6 Nov 2001 11:31 pm

Sample : gc/ms unknown

Misc :

MS Integration Params: RTEINT.P

Quant Time: Nov 7 0:19 2001

Vial: 12

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

Quant Results File: NP103001.RES

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Nov 02 16:41:16 2001

Response via : Initial Calibration

DataAcq Meth : NP103001

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	11.71	152	752545	20.00	ug/l	-0.02
19) Naphthalene-d8	15.32	136	2922047	20.00	ug/l	-0.02
31) Acenaphthene-d10	20.59	164	1465366	20.00	ug/l	-0.02
49) Phenanthrene-d10	25.02	188	2235917	20.00	ug/l	-0.02
59) Chrysene-d12	33.06	240	1589587	20.00	ug/l	0.00
68) Perylene-d12	37.17	264	1145360	20.00	ug/l	0.00

System Monitoring Compounds

4) 2-Fluorophenol	0.00	112	0	0.00	ug/l	
Spiked Amount	75.000		Recovery	=	0.00%	
5) Phenol-d5	0.00	99	0	0.00	ug/l	
Spiked Amount	75.000		Recovery	=	0.00%	
6) 2-Chlorophenol-d4	11.71	132	527	0.01	ug/l	0.47
Spiked Amount	75.000		Recovery	=	0.01%	
7) 1,2-Dichlorobenzene-d4	12.23	152	8837	0.26	ug/l	-0.02
Spiked Amount	50.000		Recovery	=	0.52%	
20) Nitrobenzene-d5	0.00	82	0	0.00	ug/l	
Spiked Amount	50.000		Recovery	=	0.00%	
32) 2-Fluorobiphenyl	18.75	172	3144	0.03	ug/l	0.13
Spiked Amount	50.000		Recovery	=	0.06%	
33) 2,4,6-Tribromophenol	0.00	330	0	0.00	ug/l	
Spiked Amount	75.000		Recovery	=	0.00%	
62) Terphenyl-d14	0.00	244	0	0.00	ug/l	
Spiked Amount	50.000		Recovery	=	0.00%	

Target Compounds

					Qvalue
2) Pyridine	0.00	79	0	N.D.	
3) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
8) Phenol	0.00	94	0	N.D.	
9) bis(2-Chloroethyl)ether	0.00	93	0	N.D.	
10) 2-Chlorophenol	0.00	128	0	N.D.	
11) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
12) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
13) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
14) 2-Methylphenol	0.00	108	0	N.D.	
15) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
16) 3&4-Methylphenol	0.00	108	0	N.D.	
17) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
18) Hexachloroethane	0.00	117	0	N.D.	
21) Nitrobenzene	0.00	77	0	N.D.	
22) Isophorone	0.00	82	0	N.D.	

(#)=qualifier out of range (m)=manual integration

24881.D NP103001.M Fri Nov 16 12:10:52 2001

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV0601\24881.D
 Acq On : 6 Nov 2001 11:31 pm
 Sample : gc/ms unknown
 Misc :
 MS Integration Params: RTEINT.P
 Quant Time: Nov 7 0:19 2001

Vial: 12
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: NP103001.RES

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Fri Nov 02 16:41:16 2001
 Response via : Initial Calibration
 DataAcq Meth : NP103001

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
23) 2-Nitrophenol	0.00	139	0	N.D.		
24) 2,4-Dimethylphenol	0.00	107	0	N.D.		
25) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.		
26) 2,4-Dichlorophenol	0.00	162	0	N.D.		
27) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.		
28) Naphthalene	0.00	128	0	N.D.		
29) Hexachlorobutadiene	0.00	225	0	N.D.		
30) 4-Chloro-3-methylphenol	0.00	107	0	N.D.		
34) Hexachlorocyclopentadiene	0.00	237	0	N.D.		
35) 2,4,6-Trichlorophenol	0.00	196	0	N.D.		
36) 2,4,5-Trichlorophenol	0.00	196	0	N.D.		
37) 2-Chloronaphthalene	0.00	162	0	N.D.		
38) Dimethylphthalate	0.00	163	0	N.D.		
39) 2,6-Dinitrotoluene	0.00	165	0	N.D.		
40) Acenaphthylene	0.00	152	0	N.D.		
41) Acenaphthene	0.00	153	0	N.D.		
42) 2,4-Dinitrophenol	0.00	184	0	N.D.		
43) 4-Nitrophenol	0.00	65	0	N.D.		
44) 2,4-Dinitrotoluene	21.10	165	181	N.D.		
45) Diethylphthalate	0.00	149	0	N.D.		
46) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.		
47) Fluorene	0.00	166	0	N.D.		
48) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.		
50) 4,6-Dinitro-2-methylphenol	0.00	198	0	N.D.		
51) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
52) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
53) Hexachlorobenzene	0.00	284	0	N.D.		
54) Pentachlorophenol	0.00	266	0	N.D.		
55) Phenanthrene	25.02	178	846	N.D.		
56) Anthracene	25.02	178	846	N.D.		
57) Di-n-butylphthalate	27.03	149	2447	N.D.		
58) Fluoranthene	0.00	202	0	N.D.		
60) 3,3'-Dichlorobenzidine	0.00	252	0	N.D.		
61) Benzidine	0.00	184	0	N.D.		
63) Pyrene	0.00	202	0	N.D.		
64) Butylbenzylphthalate	0.00	149	0	N.D.		
65) Benzo(a)anthracene	33.06	228	4047	N.D.		
66) Bis(2-ethylhexyl)phthalate	33.34	149	819	N.D.		
67) Chrysene	33.06	228	4047	N.D.		
69) Di-n-Octylphthalate	0.00	149	0	N.D.		
70) Benzo(b)fluoranthene	0.00	252	0	N.D.		

(#) = qualifier out of range (m) = manual integration
 24881.D NP103001.M Fri Nov 16 12:10:55 2001

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV0601\24881.D
 Acq On : 6 Nov 2001 11:31 pm
 Sample : gc/ms unknown
 Misc :
 MS Integration Params: RTEINT.P
 Quant Time: Nov 7 0:19 2001

Vial: 12
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: NP103001.RES

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Fri Nov 02 16:41:16 2001
 Response via : Initial Calibration
 DataAcq Meth : NP103001

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
71) Benzo(k)fluoranthene	0.00	252	0		N.D.	
72) Benzo(a)pyrene	37.17	252	4391		N.D.	
73) Indeno(1,2,3-cd)pyrene	0.00	276	0		N.D.	
74) Dibenz(a,h)anthracene	0.00	278	0		N.D.	
75) Benzo(g,h,i)perylene	0.00	276	0		N.D.	

 (#) = qualifier out of range (m) = manual integration
 24881.D NP103001.M Fri Nov 16 12:10:56 2001


Quantitation Report

Data File : C:\HPCHEM\1\DATA\NOV0601\24881.D
 Acq On : 6 Nov 2001 11:31 pm
 Sample : gc/ms unknown
 Misc :
 MS Integration Params: RTEINT.P
 Quant Time: Nov 7 0:19 2001

Vial: 12
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: NP103001.RES

Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Fri Nov 02 16:41:16 2001
 Response via : Initial Calibration

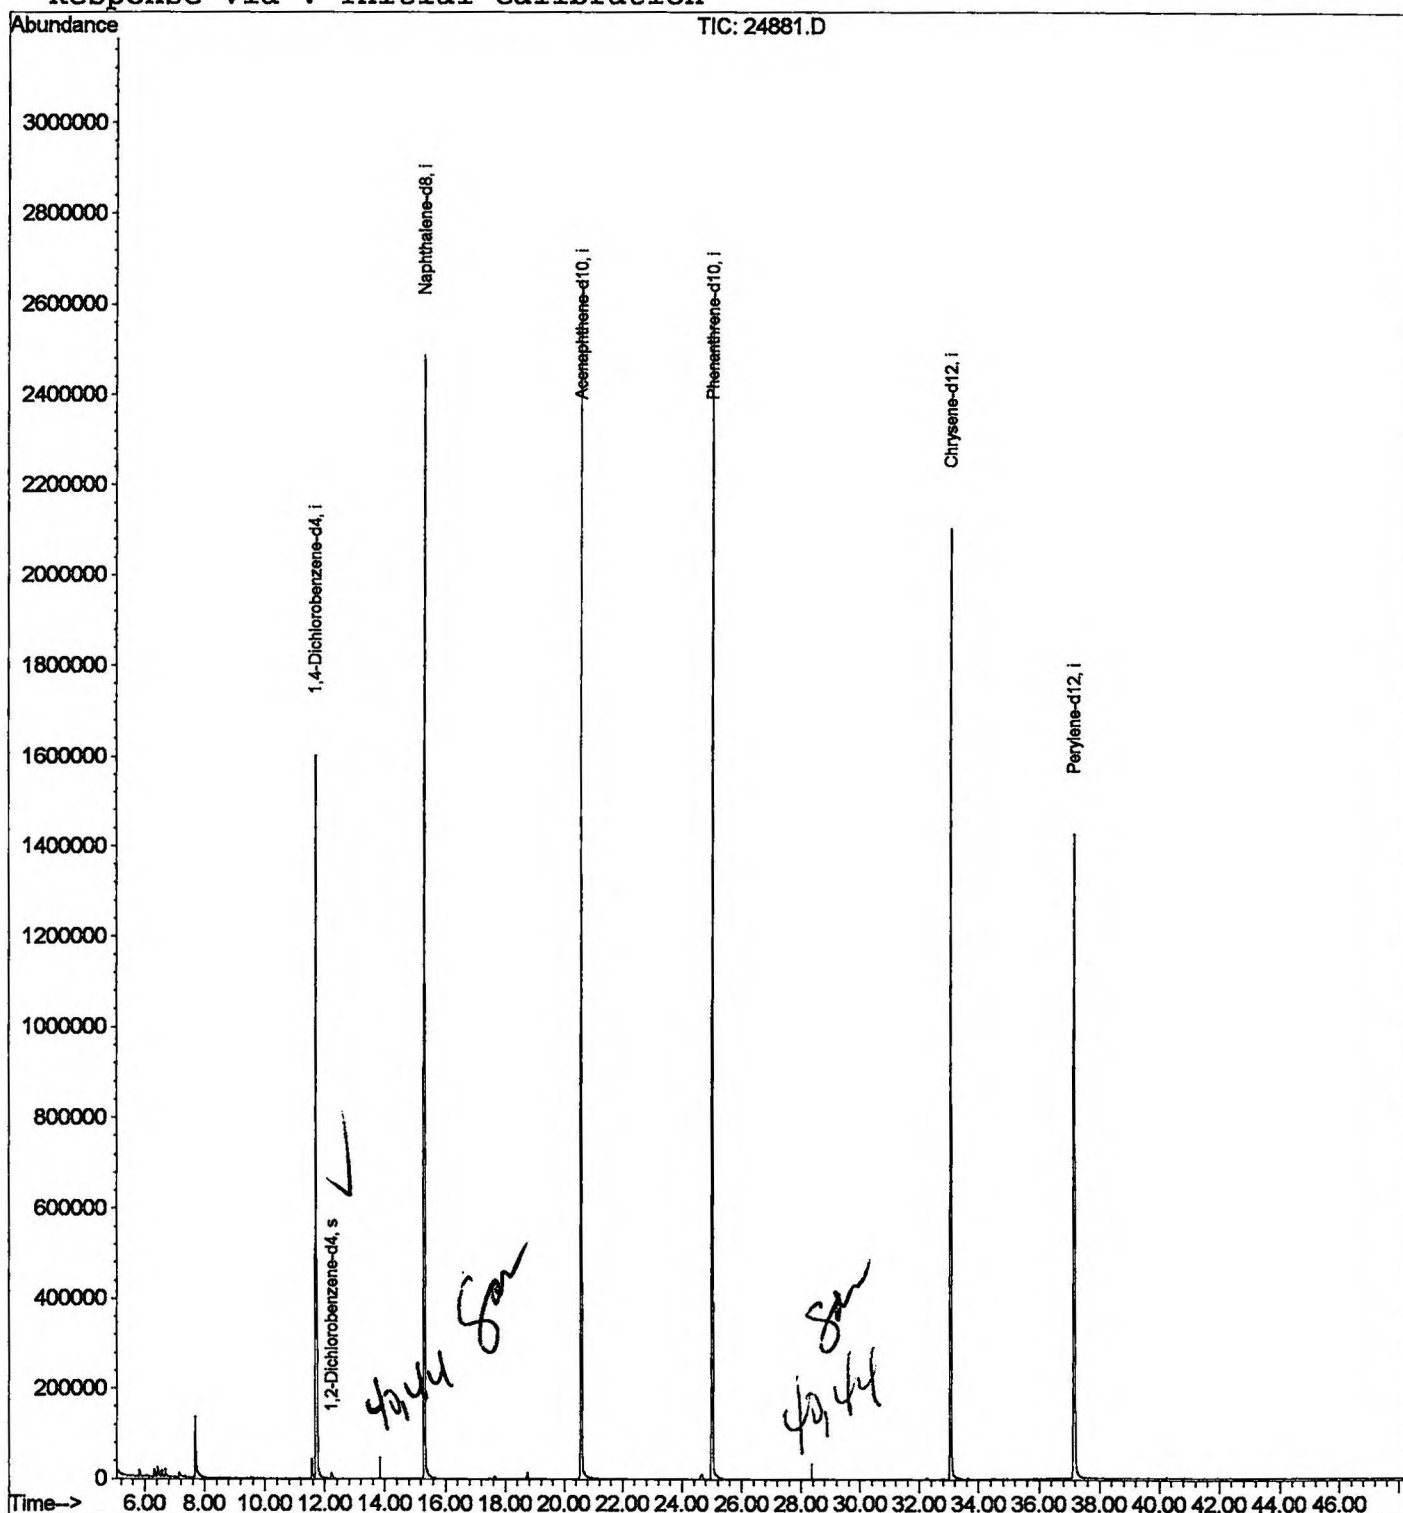

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\NOV0601\24881.D
 Acq On : 6 Nov 2001 11:31 pm
 Sample : gc/ms unknown
 Misc :
 MS Integration Params: LSCINT.P

Vial: 12
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC




peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	6.439	149	152	162	rVV	23587	61703	1.07%	0.204%
2	7.687	285	288	305	rBV	135994	372199	6.45%	1.230%
3	11.571	707	711	721	rBV	43670	104333	1.81%	0.345%
4	11.708	721	726	750	rVV	1600301	3892300	67.42%	12.861%
5	15.316	1113	1119	1137	rBV	2486438	5288987	91.61%	17.476%
6	20.595	1688	1694	1715	rBV	2652554	5773342	100.00%	19.076%
7	25.020	2169	2176	2188	rBV2	2575549	5617003	97.29%	18.559%
8	33.062	3045	3052	3071	rBV2	2102029	5015231	86.87%	16.571%
9	37.165	3490	3499	3523	rBV2	1423590	4139991	71.71%	13.679%

Sum of corrected areas: 30265089

24881.D NP103001.M Fri Nov 16 12:11:59 2001

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\NOV0601\24881.D
 Operator : 209 GALOS
 Acquired : 6 Nov 2001 11:31 pm using AcqMethod NP103001
 Instrument : GC/MS 209
 Sample Name: gc/ms unknown
 Misc Info :
 Vial Number: 12
 Quant File :NP103001.RES (RTE Integrator)

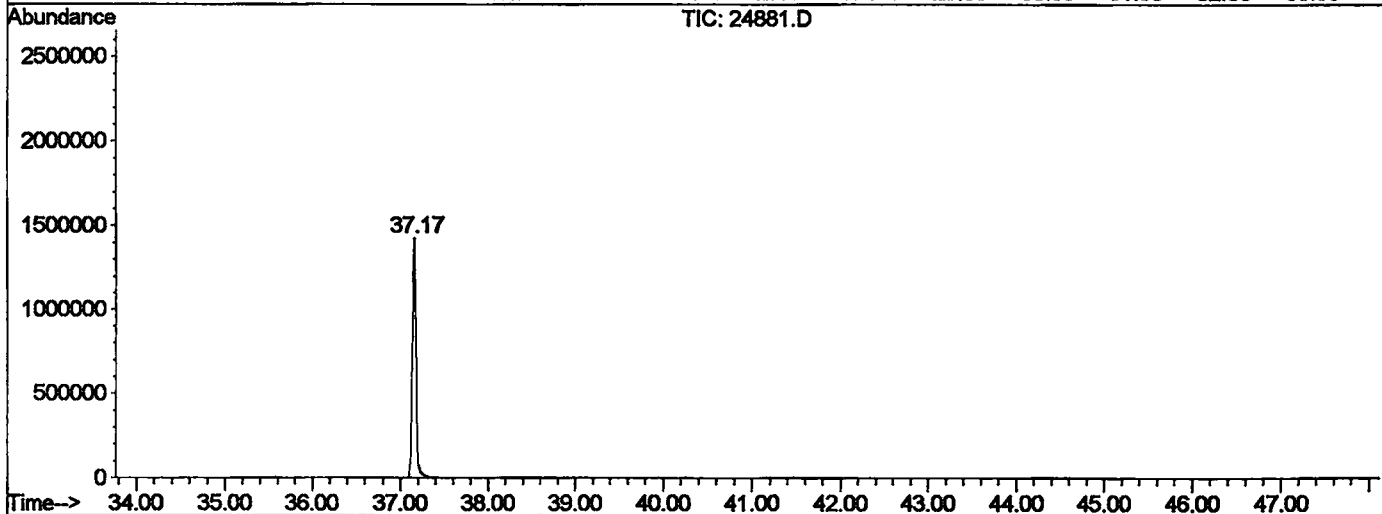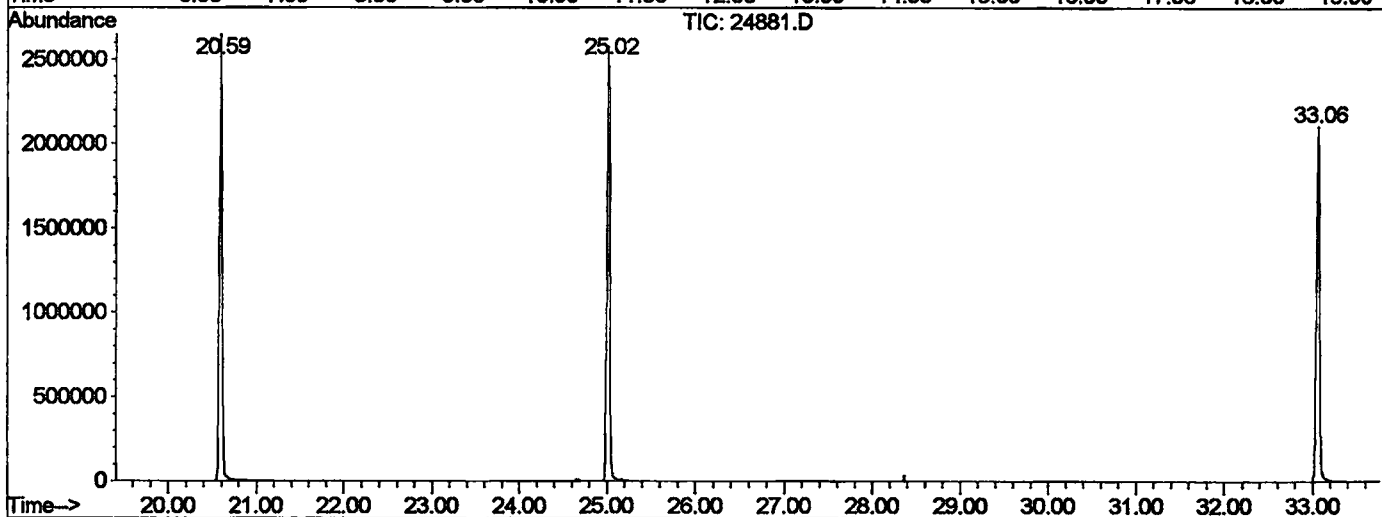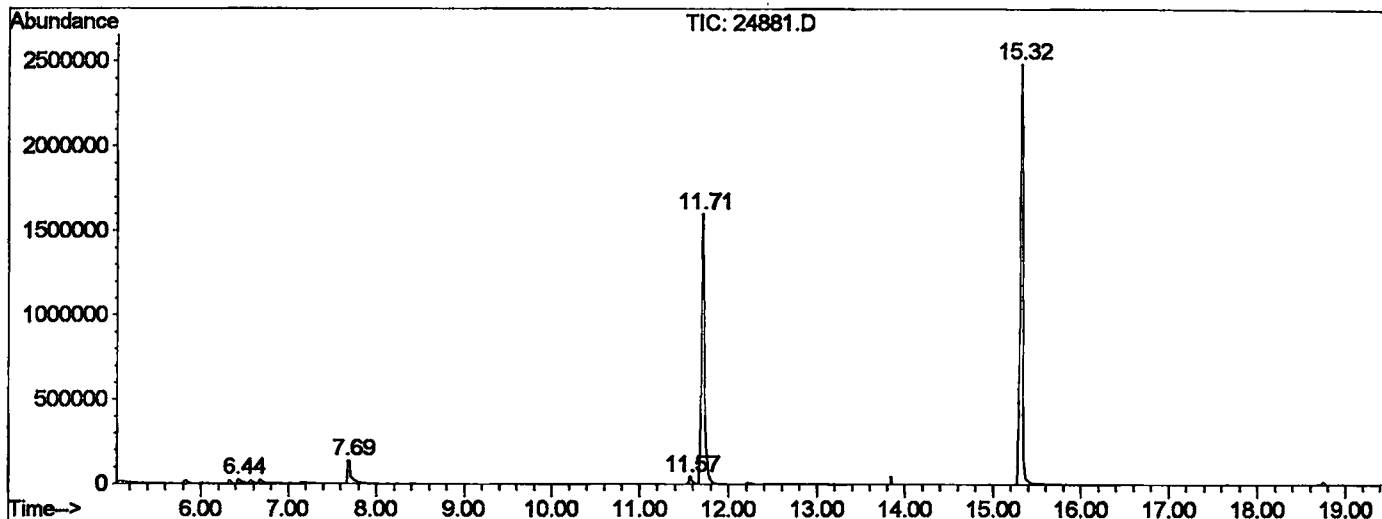

24881.D NP103001.M Fri Nov 16 12:12:01 2001

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\NOV0601\24881.D
 Acq On : 6 Nov 2001 11:31 pm
 Sample : gc/ms unknown
 Misc :
 MS Integration Params: LSCINT.P


Vial: 12
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.69	1.91 ug/l	372199	1,4-Dichlorobenzene-d4	11.71

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2			Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9
3			3-Hydroxy-2-pentanone	102	C5H10O2	003142-66-3	9
4			Acetic acid, 2-methylpropyl ester	116	C6H12O2	000110-19-0	9

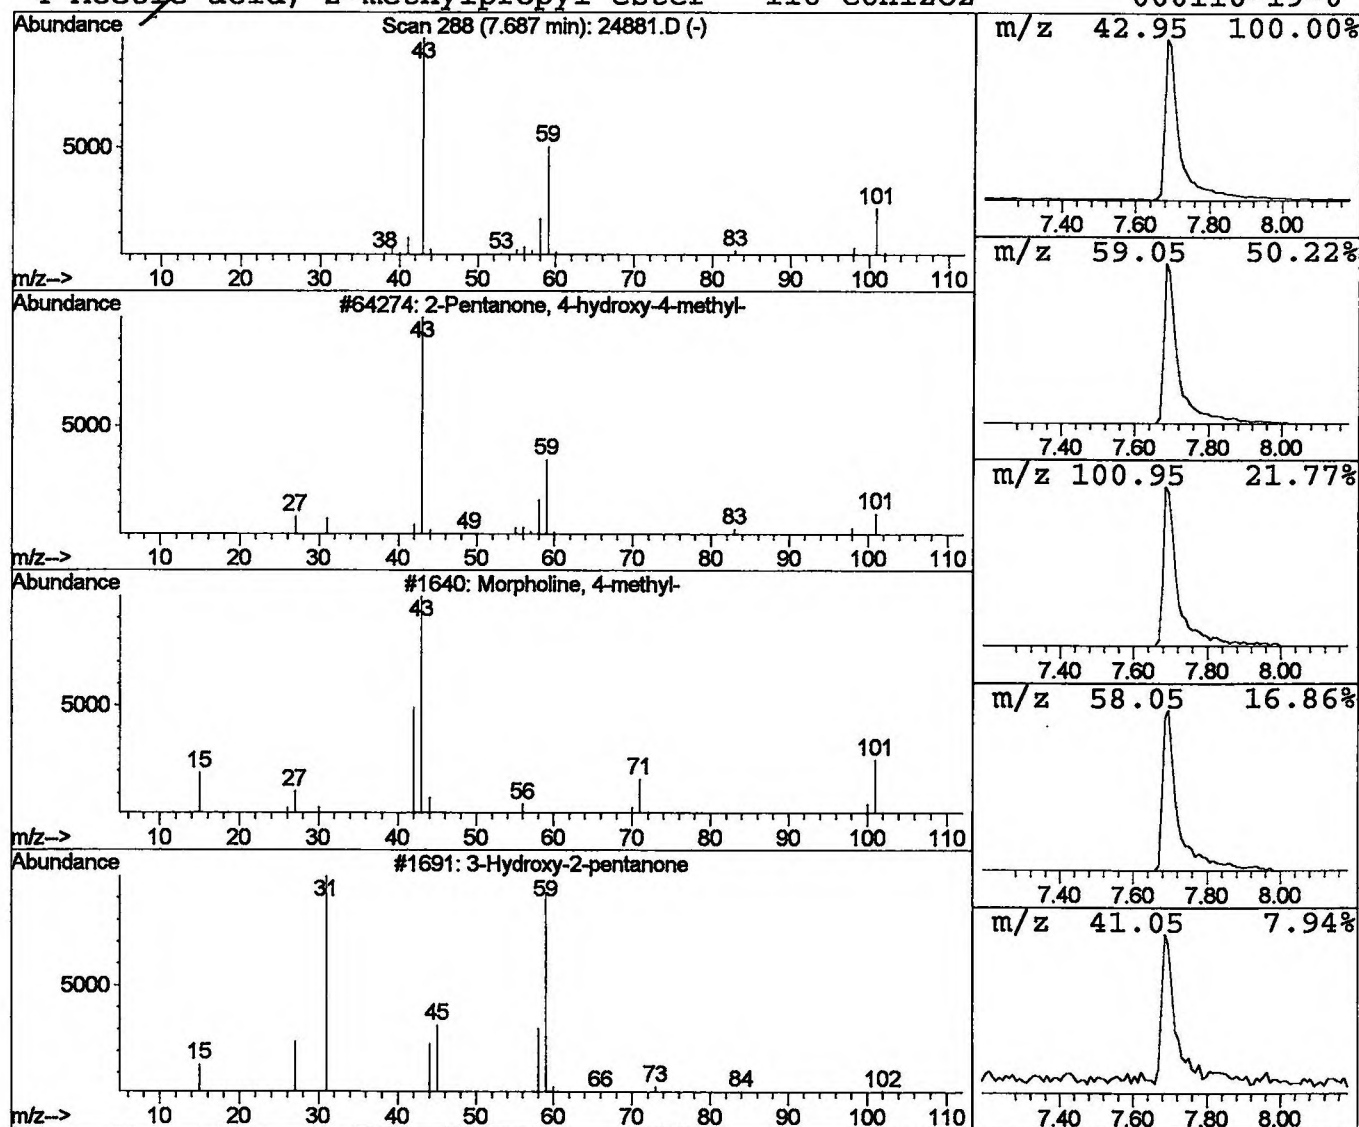

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\NOV0601\24881.D
 Acq On : 6 Nov 2001 11:31 pm
 Sample : gc/ms unknown
 Misc :
 MS Integration Params: LSCINT.P


Vial: 12
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 2 1,4-Dichlorobenzene-d4 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.57	0.54 ug/l	104333	1,4-Dichlorobenzene-d4	11.71

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1,4-Dichlorobenzene-d4	150	C6Cl2D4	003855-82-1	53
2			Benzene-1,2,3,4-d4-, 5,6-dichloro-	150	C6Cl2D4	002199-69-1	16
3			2-Methyl-6-nitroaniline	152	C7H8N2O2	000570-24-1	10
4			Benzaldehyde, 2-hydroxy-3-methoxy-	152	C8H8O3	000148-53-8	10

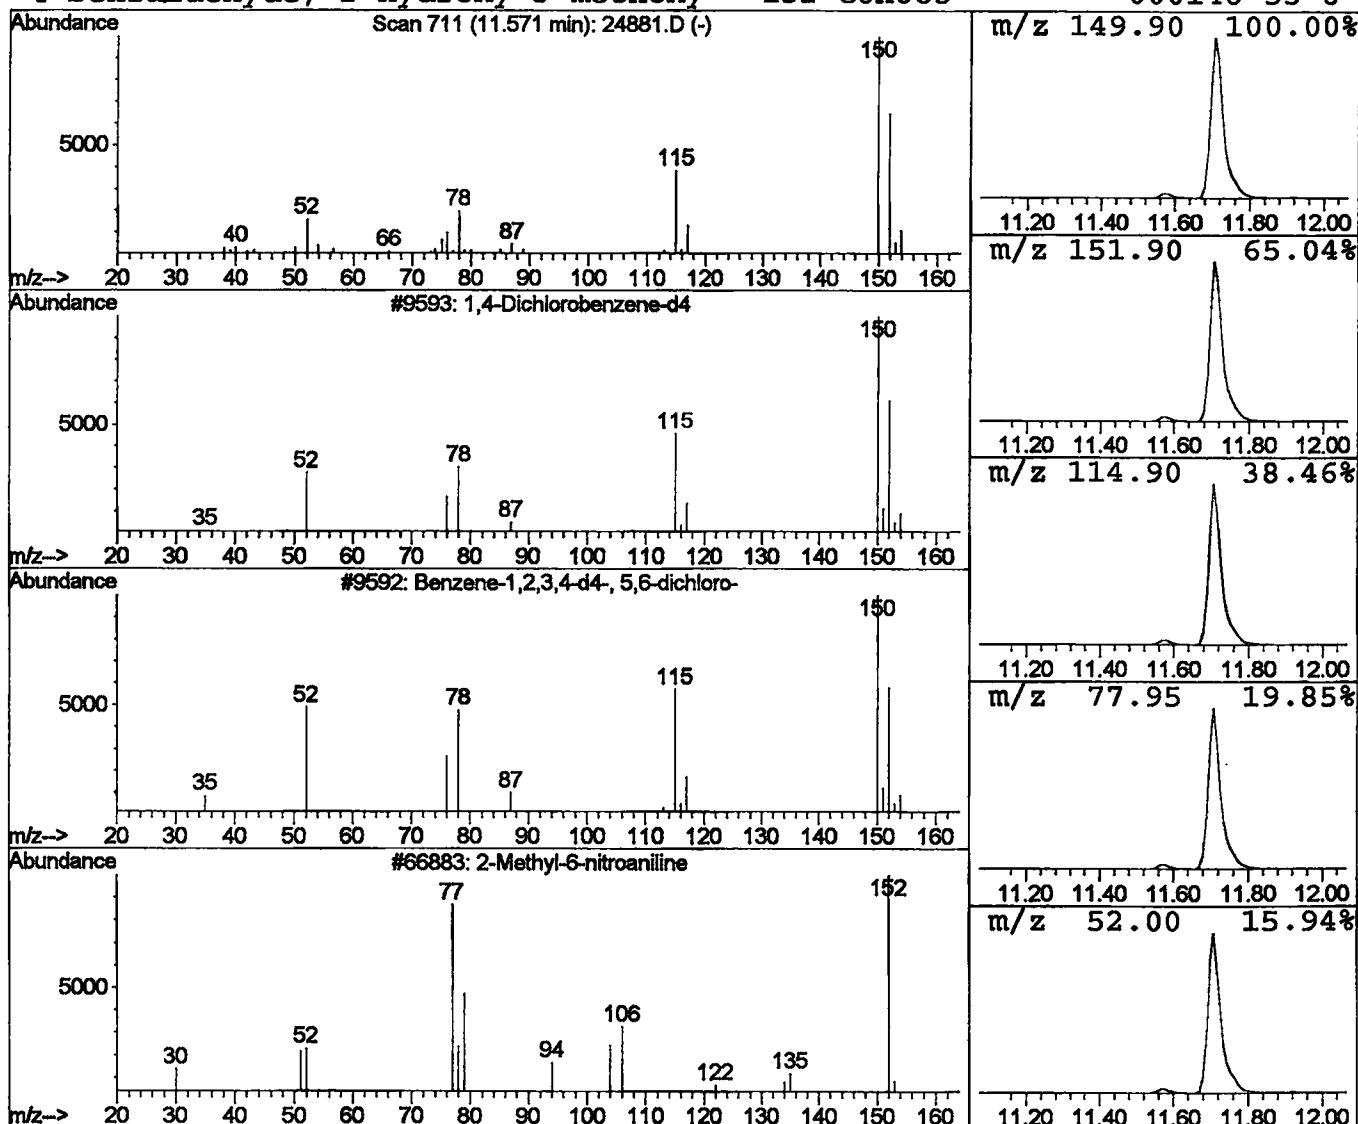

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 6 Nov 2001 11:31 pm
 Data File: C:\HPCHEM\1\DATA\NOV0601\24881.D
 Name: gc/ms unknown
 Misc:
 Method: C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	7.69	1.9	ug/l	372199	ISTD01	11.71	3892300	20.0
1,4-Dichlorobenzene-	11.57	0.5	ug/l	104333	ISTD01	11.71	3892300	20.0

24881.D NP103001.M Fri Nov 16 12:12:07 2001