

Method 508 tox + chl Date Extracted 10/19/01
 NYS samples GC MS scans

Page 38

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count
	CB	1000		1ml			2ml			
	1000 chl				✓					
	Ref chl				✓					
	1000 Tox				✓					
	Ref Tox				✓					
	1000 test				✓					
	GC chl				✓					
24822	Sample									12
24822	dupe									13
24824	Sample									14
24824	dupe									15
	24950 ✓									16
	24981 ✓									17
	25037 ✓									18
	25038 ✓									19
	25039 ✓									20
	25040 ✓									1
	25041 ✓									2
	PRL 1248									
25040	Spike chlorane									
25040	Spike chlorane									

Reviewed by [Signature] 10/19/01

Remarks

drip rate must be between 5-15 ml/min for liq-liq extractors

Extraction type - 90% final Solv. lot# 12960 NaCl lot# V32603 Na2SO4 lot# V11599

STANDARD INT STD LOG# Ver: V22630

CALIBRATION

REF/SPIKE chl: 1993; tox: 1992

MDL/MDRF

Q. CHECK post: 1209C; chl: 1209C

INT. STD.

SURROGATE 20640

LPC

ENDRIN/DDT

Analyst [Signature]
 revision 4/12/01

Verified by _____

Reviewed by [Signature]
 Date 11/21/01

Sequence Name: C:\HPCHEM\1\SEQUENCE\NOV0801.S
Comment: INST 209; 30Mx0.25umX0.50
Operator: 209 GALOS
Data Path: C:\HPCHEM\1\data\nov0801\
Pre-Seq Cmd:
Post-Seq Cmd:


Method Sections To Run	On A Barcode Mismatch
(X) Full Method	(X) Inject Anyway
() Reprocessing Only	() Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	NP103001	
2	Sample	2	LB	NP103001	10/19
3	Sample	3	25042	NP103001	gc/ms unknown
4	Sample	4	25043	NP103001	gc/ms unknown
5	Sample	5	25044	NP103001	gc/ms unknown
6	Sample	6	25047	NP103001	gc/ms unknown
7	Sample	7	25048	NP103001	gc/ms unknown
8	Sample	8	LBA	NP103001	10/19 lab blk
9	Sample	9	24980 ✓	NP103001	gc/ms unknown
10	Sample	10	24981 ✓	NP103001	gc/ms unknown
11	Sample	11	25037 ✓	NP103001	gc/ms unknown
12	Sample	12	25038 ✓	NP103001	gc/ms unknown
13	Sample	13	25039 ✓	NP103001	gc/ms unknown
14	Sample	14	25040 ✓	NP103001	gc/ms unknown
15	Sample	15	25041 ✓	NP103001	gc/ms unknown

DFTPP

Data File : C:\HPCHEM\1\DATA\NOV0801\DFTPP.D
 Acq On : 8 Nov 2001 2:37 pm
 Sample :
 Misc :
 MS Integration Params: RTEINT.P
 Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

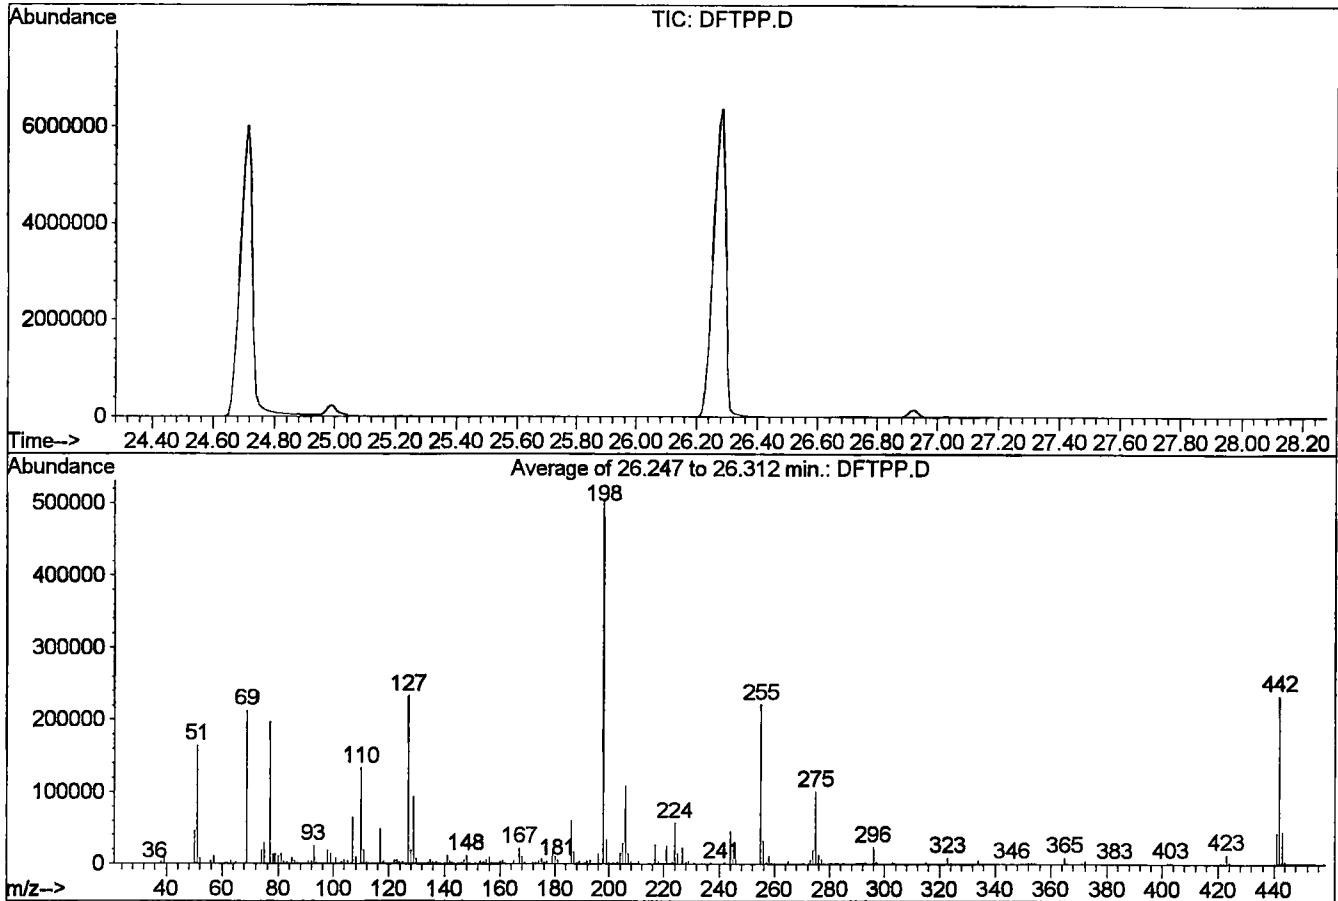

Spectrum Information: Average of 26.247 to 26.312 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	32.5	164311	PASS
68	69	0.00	2	0.0	28	PASS
69	198	0.00	100	42.1	212818	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	46.2	233532	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	505952	PASS
199	198	5	9	6.7	33773	PASS
275	198	10	30	20.1	101575	PASS
365	198	1	100	1.9	9619	PASS
441	443	0.01	100	94.5	42526	PASS
442	198	40	110	46.3	234144	PASS
443	442	17	23	19.2	45019	PASS