

User: Galos, Marie
 Westchester Dept. of Labs & Research
 Date: 11/19/2001 Time: 14:59:11

Sample: AD25039
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 11/19/01 14:57 Ended: 11/19/01 14:57 Analyst: MG
 Page: 1

	Component Name	Viol	Result
1	Other unknown compounds		see comment

*handed for
 repts.
 Rems Cpm
 10/19/01*

Comments for Sample AD25039 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Galos, Marie

Date: 11-19-2001 Time: 14:59:16

A scan of the extract prepared for the 508 analysis, from 35-550 amu using a mass spectrometer, does not reveal the presence of non-target compounds.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV0801\25039.D

Vial: 13

Acq On : 9 Nov 2001 2:19 am

Operator: 209 GALOS

Sample : gc/ms unknown

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Nov 9 3:08 2001

Quant Results File: NP103001.RES

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Nov 02 16:41:16 2001

Response via : Initial Calibration

DataAcq Meth : NP103001

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	11.71	152	960350	20.00	ug/l	-0.01
19) Naphthalene-d8	15.32	136	3747500	20.00	ug/l	-0.01
31) Acenaphthene-d10	20.60	164	1889188	20.00	ug/l	-0.01
49) Phenanthrene-d10	25.02	188	2815306	20.00	ug/l	-0.01
59) Chrysene-d12	33.06	240	2085760	20.00	ug/l	0.00
68) Perylene-d12	37.17	264	1652491	20.00	ug/l	0.00

System Monitoring Compounds

4) 2-Fluorophenol	0.00	112	0	0.00	ug/l	
Spiked Amount	75.000		Recovery	=	0.00%	
5) Phenol-d5	0.00	99	0	0.00	ug/l	
Spiked Amount	75.000		Recovery	=	0.00%	
6) 2-Chlorophenol-d4	11.70	132	722	0.01	ug/l	0.46
Spiked Amount	75.000		Recovery	=	0.01%	
7) 1,2-Dichlorobenzene-d4	12.23	152	11645	0.27	ug/l	-0.01
Spiked Amount	50.000		Recovery	=	0.54%	
20) Nitrobenzene-d5	0.00	82	0	0.00	ug/l	
Spiked Amount	50.000		Recovery	=	0.00%	
32) 2-Fluorobiphenyl	18.60	172	339	0.00	ug/l	-0.01
Spiked Amount	50.000		Recovery	=	0.00%	
33) 2,4,6-Tribromophenol	0.00	330	0	0.00	ug/l	
Spiked Amount	75.000		Recovery	=	0.00%	
62) Terphenyl-d14	29.94	244	2205	0.02	ug/l	0.00
Spiked Amount	50.000		Recovery	=	0.04%	

Target Compounds

					Qvalue
2) Pyridine	0.00	79	0	N.D.	
3) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
8) Phenol	0.00	94	0	N.D.	
9) bis(2-Chloroethyl)ether	0.00	93	0	N.D.	
10) 2-Chlorophenol	0.00	128	0	N.D.	
11) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
12) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
13) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
14) 2-Methylphenol	0.00	108	0	N.D.	
15) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
16) 3&4-Methylphenol	0.00	108	0	N.D.	
17) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
18) Hexachloroethane	0.00	117	0	N.D.	
21) Nitrobenzene	0.00	77	0	N.D.	
22) Isophorone	0.00	82	0	N.D.	

(#)= qualifier out of range (m)= manual integration

25039.D NP103001.M

Mon Nov 19 14:33:52 2001

Page 1

Quantitation Report (QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV0801\25039.D

Vial: 13

Acq On : 9 Nov 2001 2:19 am

Operator: 209 GALOS

Sample : gc/ms unknown

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Nov 9 3:08 2001

Quant Results File: NP103001.RES

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Nov 02 16:41:16 2001

Response via : Initial Calibration

DataAcq Meth : NP103001

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
23) 2-Nitrophenol	0.00	139	0	N.D.		
24) 2,4-Dimethylphenol	0.00	107	0	N.D.		
25) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.		
26) 2,4-Dichlorophenol	0.00	162	0	N.D.		
27) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.		
28) Naphthalene	15.36	128	1061	N.D.		
29) Hexachlorobutadiene	0.00	225	0	N.D.		
30) 4-Chloro-3-methylphenol	0.00	107	0	N.D.		
34) Hexachlorocyclopentadiene	0.00	237	0	N.D.		
35) 2,4,6-Trichlorophenol	0.00	196	0	N.D.		
36) 2,4,5-Trichlorophenol	0.00	196	0	N.D.		
37) 2-Chloronaphthalene	0.00	162	0	N.D.		
38) Dimethylphthalate	0.00	163	0	N.D.		
39) 2,6-Dinitrotoluene	0.00	165	0	N.D.		
40) Acenaphthylene	0.00	152	0	N.D.		
41) Acenaphthene	0.00	153	0	N.D.		
42) 2,4-Dinitrophenol	0.00	184	0	N.D.		
43) 4-Nitrophenol	0.00	65	0	N.D.		
44) 2,4-Dinitrotoluene	21.02	165	310	N.D.		
45) Diethylphthalate	0.00	149	0	N.D.		
46) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.		
47) Fluorene	0.00	166	0	N.D.		
48) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.		
50) 4,6-Dinitro-2-methylphenol	0.00	198	0	N.D.		
51) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
52) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
53) Hexachlorobenzene	0.00	284	0	N.D.		
54) Pentachlorophenol	0.00	266	0	N.D.		
55) Phenanthrene	25.02	178	1568	N.D.		
56) Anthracene	25.08	178	618	N.D.		
57) Di-n-butylphthalate	27.02	149	3276	N.D.		
58) Fluoranthene	0.00	202	0	N.D.		
60) 3,3'-Dichlorobenzidine	0.00	252	0	N.D.		
61) Benzidine	0.00	184	0	N.D.		
63) Pyrene	0.00	202	0	N.D.		
64) Butylbenzylphthalate	0.00	149	0	N.D.		
65) Benzo(a)anthracene	33.06	228	4984	N.D.		
66) Bis(2-ethylhexyl)phthalate	33.32	149	1445	N.D.		
67) Chrysene	33.06	228	4984	N.D.		
69) Di-n-Octylphthalate	0.00	149	0	N.D.		
70) Benzo(b)fluoranthene	0.00	252	0	N.D.		

(#)=qualifier out of range (m)=manual integration

25039.D NP103001.M Mon Nov 19 14:33:57 2001

Page 2

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV0801\25039.D

Vial: 13

Acq On : 9 Nov 2001 2:19 am

Operator: 209 GALOS

Sample : gc/ms unknown

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Nov 9 3:08 2001

Quant Results File: NP103001.RES

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Nov 02 16:41:16 2001

Response via : Initial Calibration

DataAcq Meth : NP103001

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
71) Benzo(k)fluoranthene	0.00	252	0	N.D.		
72) Benzo(a)pyrene	37.17	252	6322	N.D.		
73) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
74) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
75) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

25039.D NP103001.M Mon Nov 19 14:33:59 2001

Page 3


Quantitation Report

Data File : C:\HPCHEM\1\DATA\NOV0801\25039.D
Acq On : 9 Nov 2001 2:19 am
Sample : gc/ms unknown
Misc :
MS Integration Params: RTEINT.P
Quant Time: Nov 9 3:08 2001

Vial: 13
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: NP103001.RES

Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Fri Nov 02 16:41:16 2001
Response via : Initial Calibration

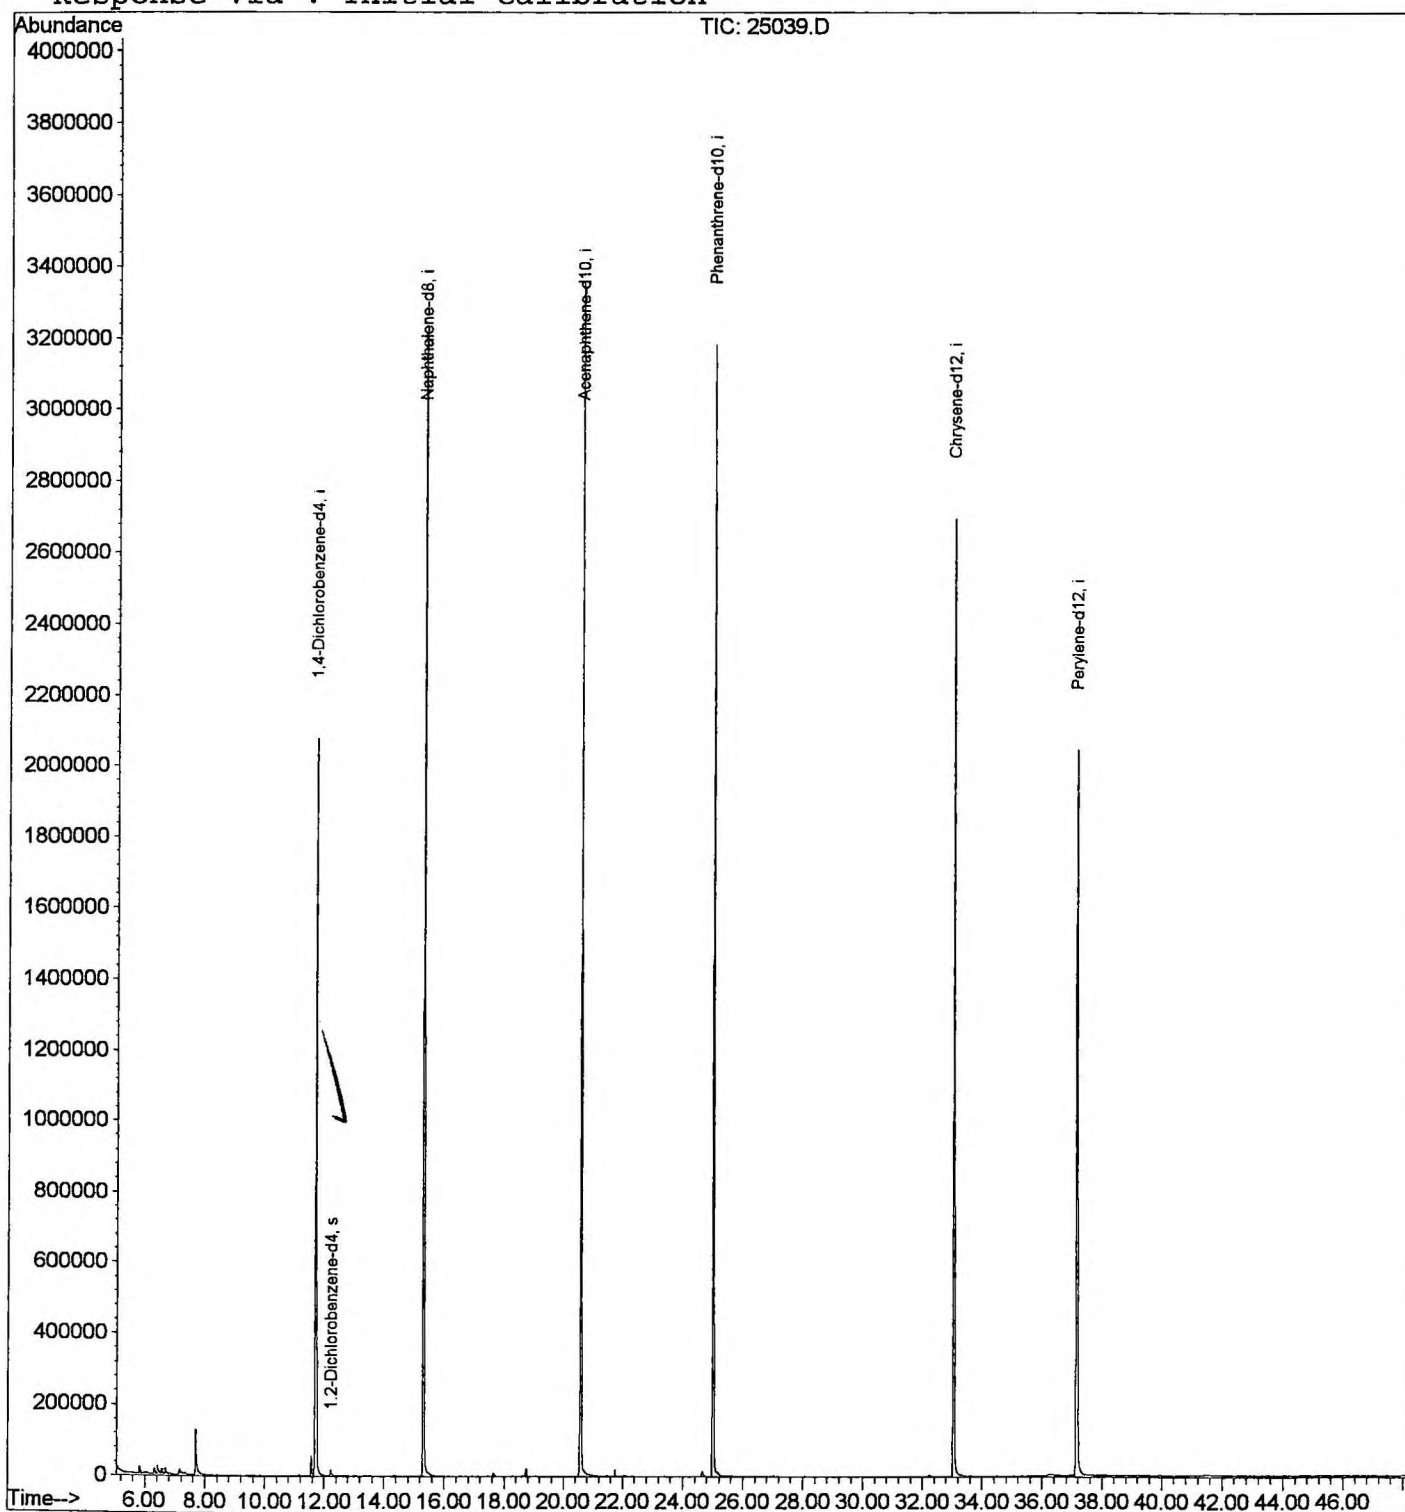

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\NOV0801\25039.D

Acq On : 9 Nov 2001 2:19 am

Sample : gc/ms unknown

Misc :

MS Integration Params: LSCINT.P

Vial: 13

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	7.689	285	288	305	rBV	128185	348246	4.71%	0.890%
2	11.572	706	711	721	rBV	57669	135467	1.83%	0.346%
3	11.710	721	726	742	rVV	2072846	4942879	66.82%	12.632%
4	15.318	1113	1119	1137	rBV	3212399	6807997	92.03%	17.398%
5	20.596	1687	1694	1719	rBV	3360478	7397541	100.00%	18.905%
6	25.021	2169	2176	2189	rBV2	3180667	7042033	95.19%	17.996%
7	33.063	3044	3052	3064	rBV2	2694966	6506550	87.96%	16.628%
8	37.167	3489	3499	3521	rBV	2044091	5949560	80.43%	15.204%


Sum of corrected areas: 39130273

25039.D NP103001.M

Mon Nov 19 14:35:45 2001

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\NOV0801\25039.D
 Operator : 209 GALOS
 Acquired : 9 Nov 2001 2:19 am using AcqMethod NP103001
 Instrument : GC/MS 209
 Sample Name: gc/ms unknown
 Misc Info :
 Vial Number: 13
 Quant File :NP103001.RES (RTE Integrator)

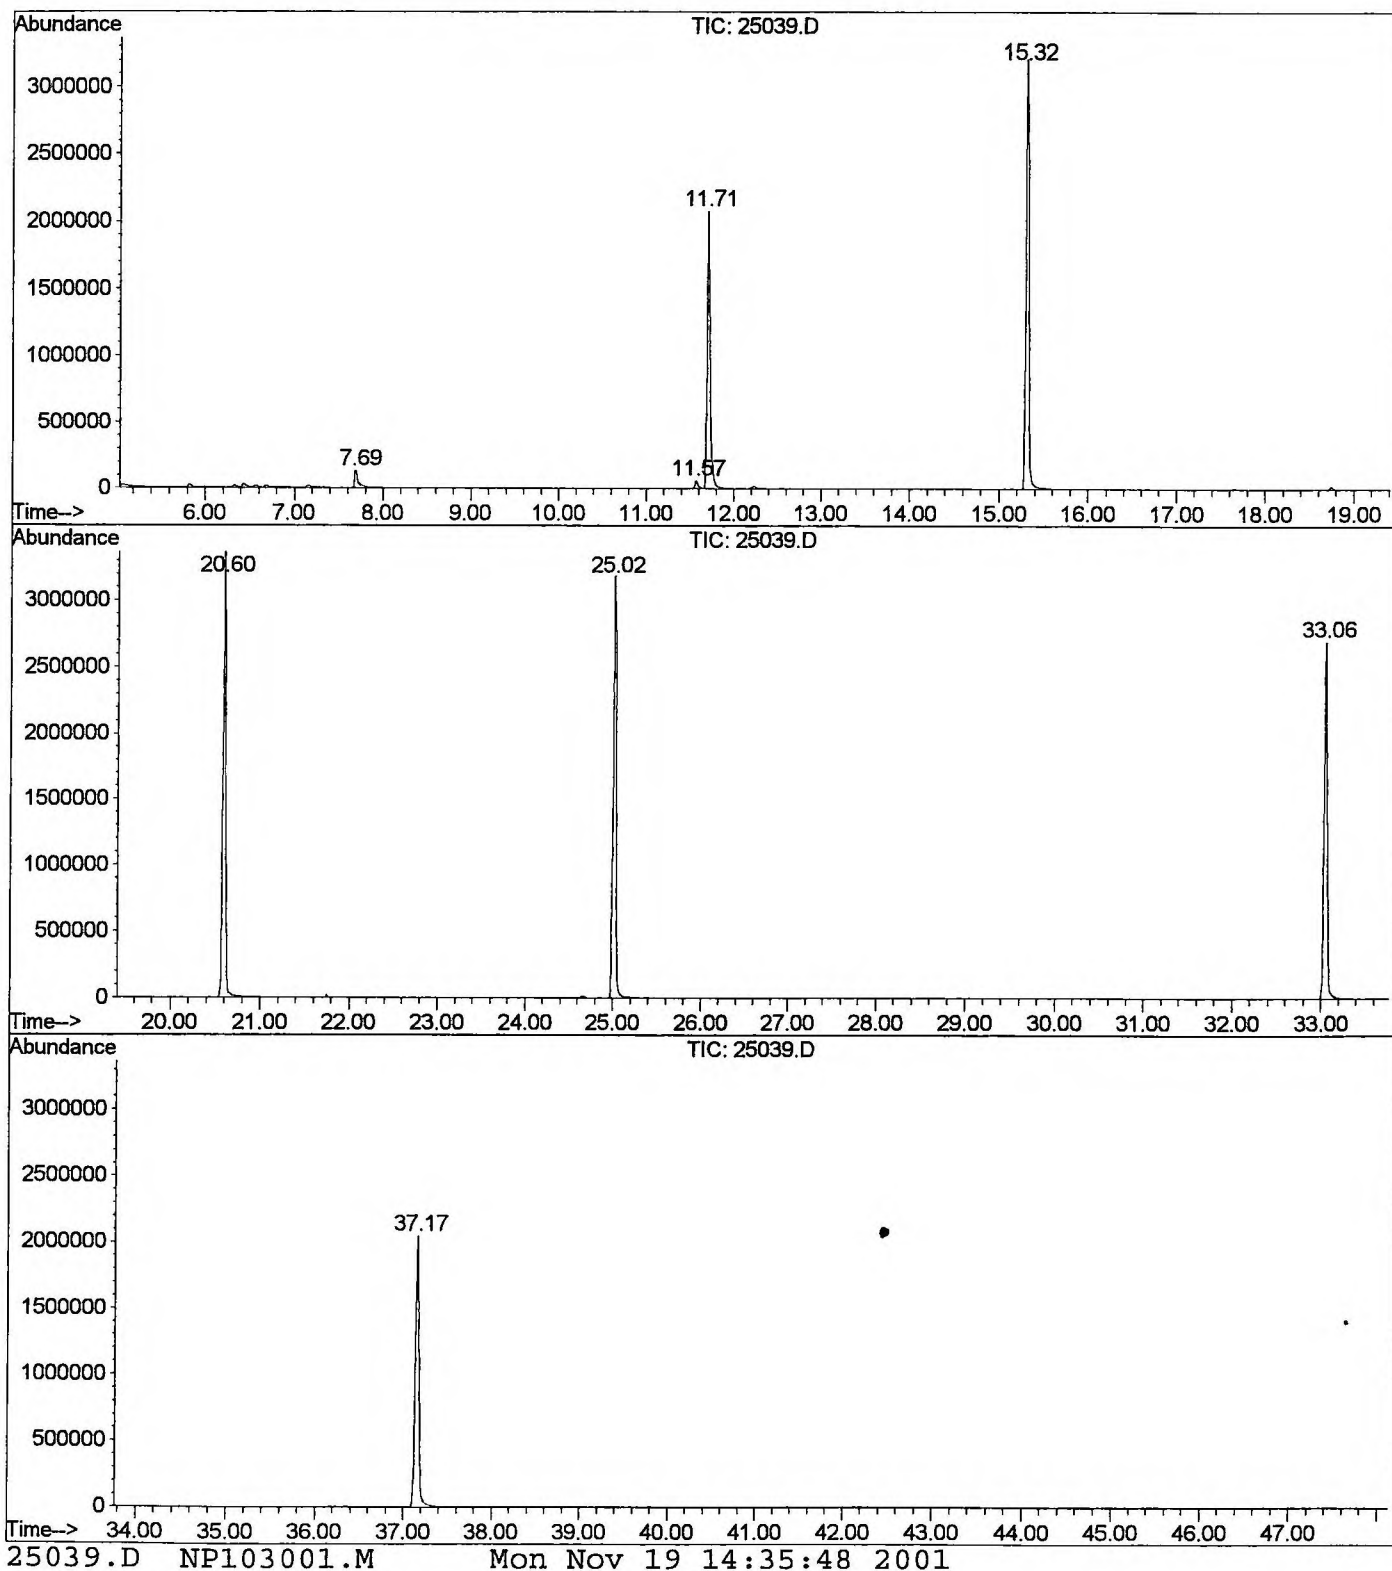

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\NOV0801\25039.D
 Acq On : 9 Nov 2001 2:19 am
 Sample : gc/ms unknown
 Misc :
 MS Integration Params: LSCINT.P


Vial: 13
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 2-Pentanone, 4-hydroxy-4-methyl Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.69	1.41 ug/l	348246	1,4-Dichlorobenzene-d4	11.71

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	72
2		5-Hexen-2-one	98	C6H10O	000109-49-9	9
3		3-Hydroxy-2-pentanone	102	C5H10O2	003142-66-3	9
4		Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9

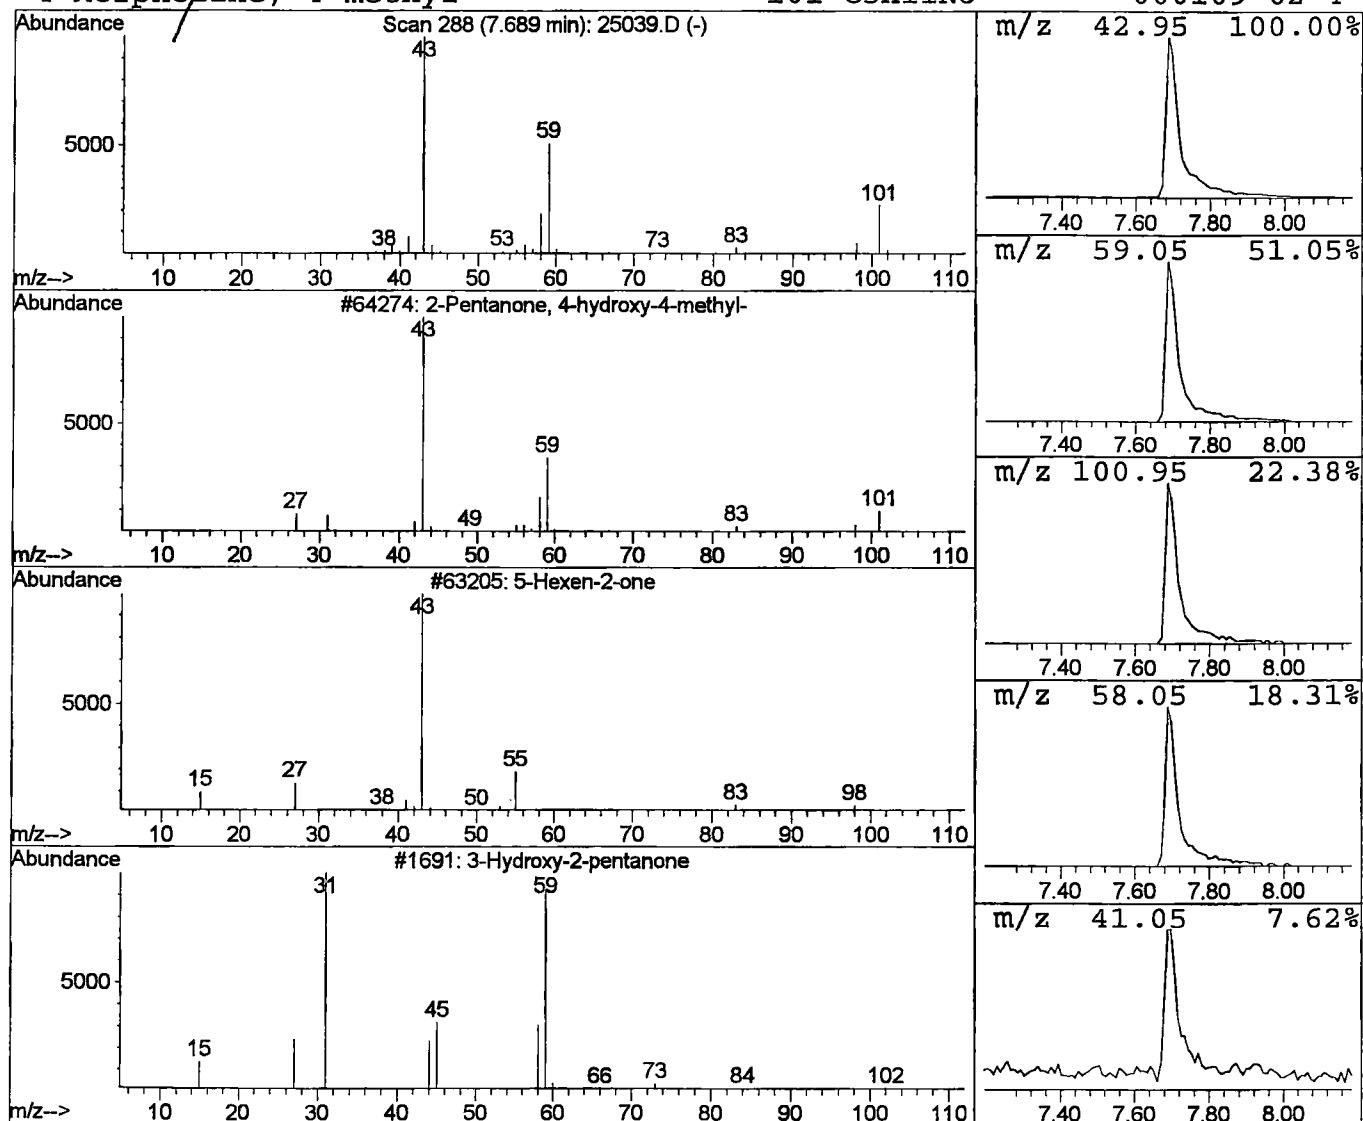

Library Search Compound Report


Data File : C:\HPCHEM\1\DATA\NOV0801\25039.D
Acq On : 9 Nov 2001 2:19 am
Sample : gc/ms unknown
Misc :
MS Integration Params: LSCINT.P

Vial: 13
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 2 1,4-Dichlorobenzene-d4 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.		
11.57	0.55 ug/l	135467	1,4-Dichlorobenzene-d4	11.71		
Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1,4-Dichlorobenzene-d4	150	C6Cl2D4	003855-82-1	58
2		Benzene-1,2,3,4-d4-, 5,6-dichloro-	150	C6Cl2D4	002199-69-1	16
3		Cyclopentanone, 2-cyclopentylidene-	150	C10H14O	000825-25-2	9
4		Benzaldehyde, 2-hydroxy-5-methoxy-	152	C8H8O3	000672-13-9	9

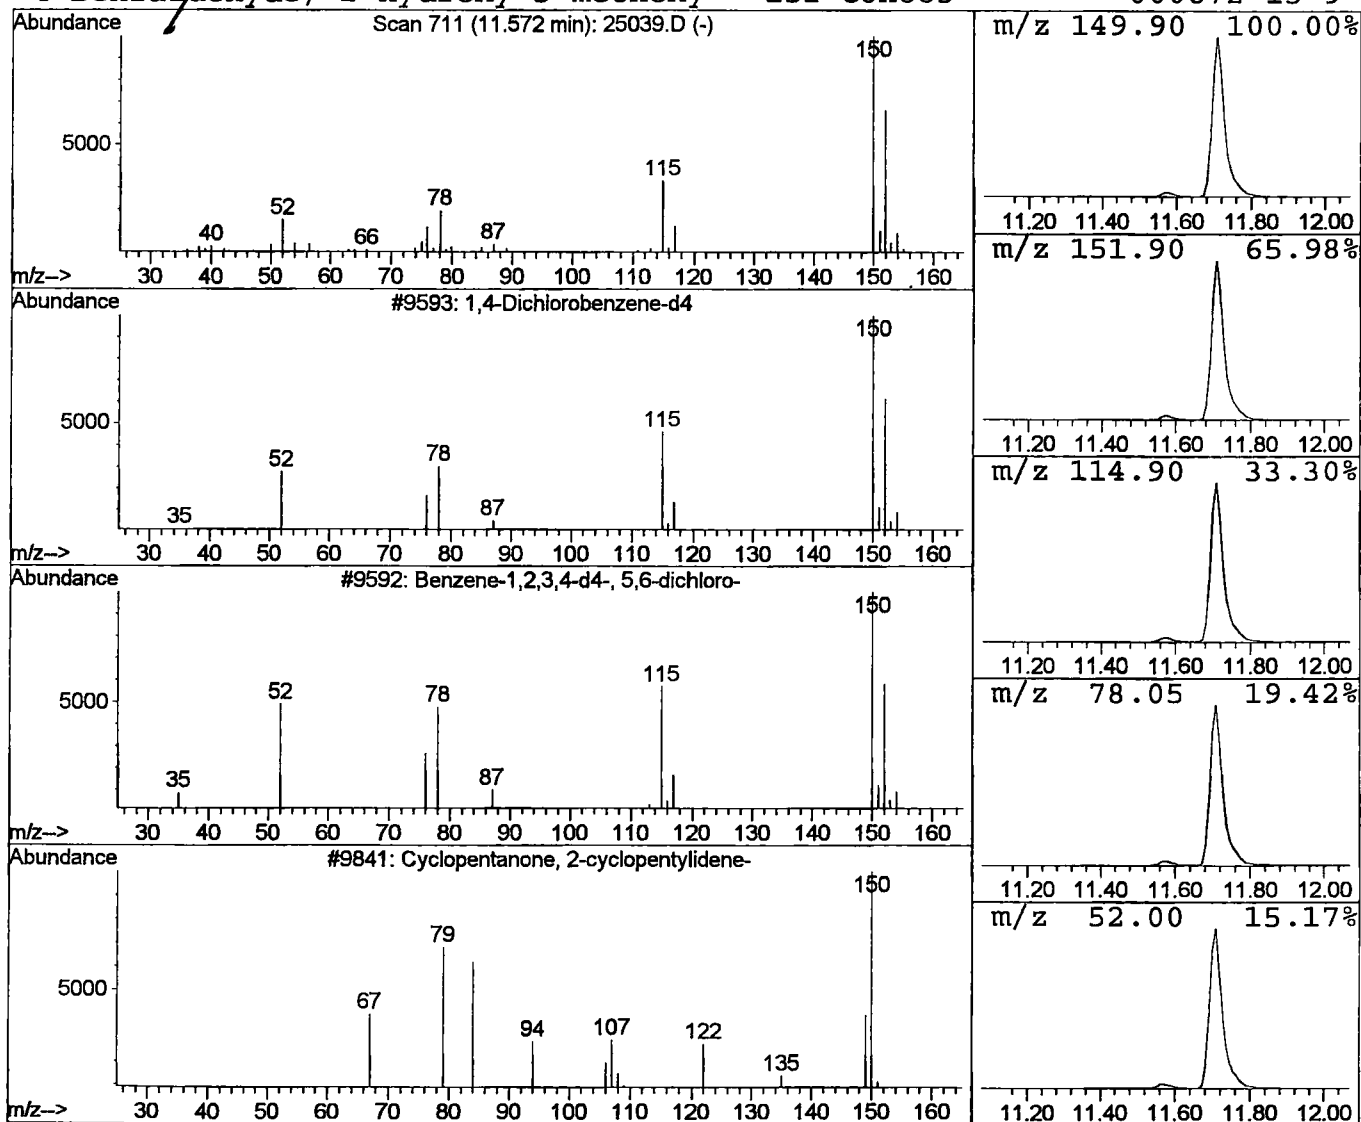

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 9 Nov 2001 2:19 am
Data File: C:\HPCHEM\1\DATA\NOV0801\25039.D
Name: gc/ms unknown
Misc:
Method: C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	7.69	1.4	ug/l	348246	ISTD01	11.71	4942880	20.0
1,4-Dichlorobenzene-	11.57	0.5	ug/l	135467	ISTD01	11.71	4942880	20.0

25039.D NP103001.M Mon Nov 19 14:35:55 2001