

Method 508Date Extracted 10/22/01Page 42Refms

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
	labbly 500ml		—	1ml	—	—	2ml		=7			
	MDL chla											
	Reference chla											
	PRL 1254											
	25042									3		
	25043									4		
	25044									5		
	25045									6		
	25047									7		
	25048									8		
Reviewed by, <u>9/21/02</u>												
Remarks 25045 sent to Engress												
drip rate must be between 5-15 ml/min for liq-liq extractors drip rate -												
Extraction type - <u>Septum</u>		Solv. lot#		NaCl lot#		Na2SO4 lot#						
STANDARD	INT STD LOG#											
CALIBRATION												
REF/SPIKE	1993	PRL1254 - 1505										
MDL/MDRF	1993											
Q. CHECK												
INT. STD.												
SURROGATE	20646											
LPC												
ENDRIN/DDT												

Analyst My/AD
revision 4/12/01

Verified by _____

Reviewed by DN
Date 12/4/01

Sequence Name: C:\HPCHEM\1\SEQUENCE\NOV0801.S
Comment: INST 209; 30Mx0.25umX0.50
Operator: 209 GALOS
Data Path: C:\HPCHEM\1\data\nov0801\
Pre-Seq Cmd:
Post-Seq Cmd:

Method Sections To Run On A Barcode Mismatch
(X) Full Method (X) Inject Anyway
() Reprocessing Only () Don't Inject

Line Type	Vial	DataFile	Method	Sample Name
1 Sample	1	DFTPP	NP103001	
2 Sample	2	LB	NP103001	10/19 22 my report
3 Sample	3	25042	NP103001	gc/ms unknown
4 Sample	4	25043	NP103001	gc/ms unknown
5 Sample	5	25044	NP103001	gc/ms unknown
6 Sample	6	25047	NP103001	gc/ms unknown
7 Sample	7	25048	NP103001	gc/ms unknown
8 Sample	8	LBA	NP103001	10/19 lab blk
9 Sample	9	24980	NP103001	gc/ms unknown
10 Sample	10	24981	NP103001	gc/ms unknown
11 Sample	11	25037	NP103001	gc/ms unknown
12 Sample	12	25038	NP103001	gc/ms unknown
13 Sample	13	25039	NP103001	gc/ms unknown
14 Sample	14	25040	NP103001	gc/ms unknown
15 Sample	15	25041	NP103001	gc/ms unknown

DFTPP

Data File : C:\HPCHEM\1\DATA\NOV0801\DFTPP.D

Acq On : 8 Nov 2001 2:37 pm

Sample :

Misc :

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

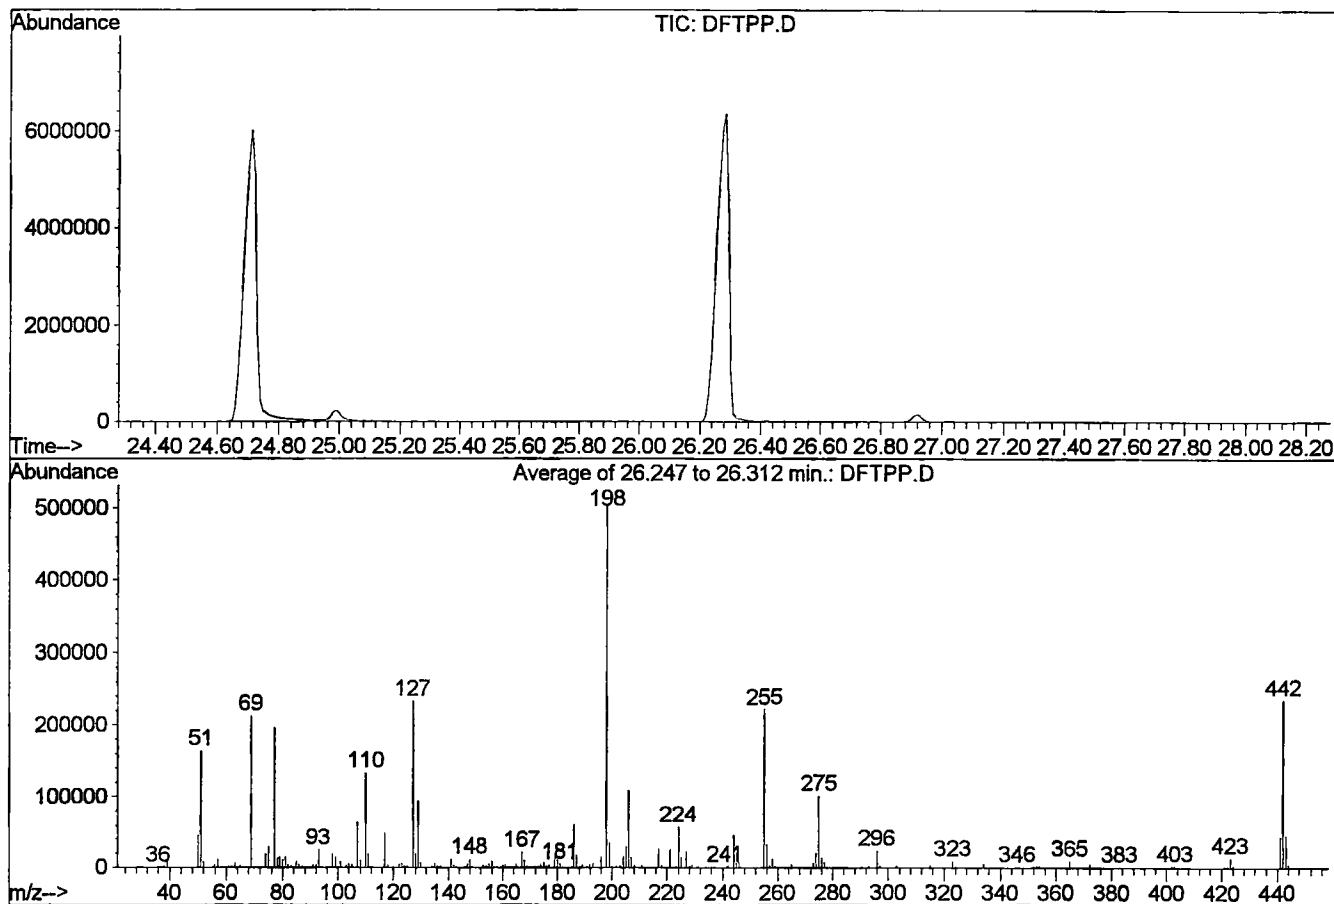

Spectrum Information: Average of 26.247 to 26.312 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	32.5	164311	PASS
68	69	0.00	2	0.0	28	PASS
69	198	0.00	100	42.1	212818	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	46.2	233532	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	505952	PASS
199	198	5	9	6.7	33773	PASS
275	198	10	30	20.1	101575	PASS
365	198	1	100	1.9	9619	PASS
441	443	0.01	100	94.5	42526	PASS
442	198	40	110	46.3	234144	PASS
443	442	17	23	19.2	45019	PASS

DFTPP.D NP103001.M

Mon Nov 19 11:55:46 2001