

User: Galos, Marie
 Westchester Dept. of Labs & Research
 Date: 11/27/2001 Time: 10:38:15

Sample: AD25048
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 11/27/01 10:37 Ended: 11/27/01 10:37 Analyst: MG
 Page: 1

	Component Name	Vol	Result
1	Other unknown compounds		see comment

Comments for Sample AD25048 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Galos, Marie

Date: 11-27-2001 Time: 10:38:20

A scan of the extract prepared for the 508 analysis, from 35-550 amu using a mass spectrometer, does not reveal the presence of non-target compounds.

Quantitation Report (QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV0801\25048.D

Vial: 7

Acq On : 8 Nov 2001 8:28 pm

Operator: 209 GALOS

Sample : gc/ms unknown

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Nov 8 21:17 2001

Quant Results File: NP103001.RES

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Nov 02 16:41:16 2001

Response via : Initial Calibration

DataAcq Meth : NP103001

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	11.71	152	987387	20.00	ug/l	-0.02
19) Naphthalene-d8	15.31	136	3867952	20.00	ug/l	-0.02
31) Acenaphthene-d10	20.60	164	1970481	20.00	ug/l	0.00
49) Phenanthrene-d10	25.02	188	2897071	20.00	ug/l	-0.02
59) Chrysene-d12	33.06	240	1911590	20.00	ug/l	0.00
68) Perylene-d12	37.16	264	1460631	20.00	ug/l	0.00

System Monitoring Compounds

4) 2-Fluorophenol	0.00	112	0	0.00	ug/l	
Spiked Amount 75.000			Recovery =	0.00%		
5) Phenol-d5	0.00	99	0	0.00	ug/l	
Spiked Amount 75.000			Recovery =	0.00%		
6) 2-Chlorophenol-d4	11.71	132	458	0.01	ug/l	0.47
Spiked Amount 75.000			Recovery =	0.01%		
7) 1,2-Dichlorobenzene-d4	12.23	152	11371	0.25	ug/l	-0.02
Spiked Amount 50.000			Recovery =	0.50%		
20) Nitrobenzene-d5	0.00	82	0	0.00	ug/l	
Spiked Amount 50.000			Recovery =	0.00%		
32) 2-Fluorobiphenyl	18.74	172	4111	0.03	ug/l	0.12
Spiked Amount 50.000			Recovery =	0.06%		
33) 2,4,6-Tribromophenol	0.00	330	0	0.00	ug/l	
Spiked Amount 75.000			Recovery =	0.00%		
62) Terphenyl-d14	0.00	244	0	0.00	ug/l	
Spiked Amount 50.000			Recovery =	0.00%		

Target Compounds

						Qvalue
2) Pyridine	0.00	79	0	N.D.		
3) N-nitroso-dimethyl amine	0.00	74	0	N.D.		
8) Phenol	11.31	94	125	N.D.		
9) bis(2-Chloroethyl) ether	0.00	93	0	N.D.		
10) 2-Chlorophenol	0.00	128	0	N.D.		
11) 1,3-Dichlorobenzene	0.00	146	0	N.D.		
12) 1,4-Dichlorobenzene	0.00	146	0	N.D.		
13) 1,2-Dichlorobenzene	0.00	146	0	N.D.		
14) 2-Methylphenol	0.00	108	0	N.D.		
15) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.		
16) 3&4-Methylphenol	0.00	108	0	N.D.		
17) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.		
18) Hexachloroethane	0.00	117	0	N.D.		
21) Nitrobenzene	0.00	77	0	N.D.		
22) Isophorone	0.00	82	0	N.D.		

(#)=qualifier out of range (m)=manual integration

25048.D NP103001.M Mon Nov 19 15:04:03 2001

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV0801\25048.D

Vial: 7

Acq On : 8 Nov 2001 8:28 pm

Operator: 209 GALOS

Sample : gc/ms unknown

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Nov 8 21:17 2001

Quant Results File: NP103001.RES

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Nov 02 16:41:16 2001

Response via : Initial Calibration

DataAcq Meth : NP103001

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
23) 2-Nitrophenol	0.00	139	0	N.D.		
24) 2,4-Dimethylphenol	0.00	107	0	N.D.		
25) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.		
26) 2,4-Dichlorophenol	0.00	162	0	N.D.		
27) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.		
28) Naphthalene	0.00	128	0	N.D.		
29) Hexachlorobutadiene	0.00	225	0	N.D.		
30) 4-Chloro-3-methylphenol	0.00	107	0	N.D.		
34) Hexachlorocyclopentadiene	0.00	237	0	N.D.		
35) 2,4,6-Trichlorophenol	0.00	196	0	N.D.		
36) 2,4,5-Trichlorophenol	0.00	196	0	N.D.		
37) 2-Chloronaphthalene	0.00	162	0	N.D.		
38) Dimethylphthalate	0.00	163	0	N.D.		
39) 2,6-Dinitrotoluene	0.00	165	0	N.D.		
40) Acenaphthylene	0.00	152	0	N.D.		
41) Acenaphthene	0.00	153	0	N.D.		
42) 2,4-Dinitrophenol	0.00	184	0	N.D.		
43) 4-Nitrophenol	0.00	65	0	N.D.		
44) 2,4-Dinitrotoluene	21.15	165	110	N.D.		
45) Diethylphthalate	22.10	149	317	N.D.		
46) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.		
47) Fluorene	0.00	166	0	N.D.		
48) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.		
50) 4,6-Dinitro-2-methylphenol	0.00	198	0	N.D.		
51) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
52) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
53) Hexachlorobenzene	0.00	284	0	N.D.		
54) Pentachlorophenol	0.00	266	0	N.D.		
55) Phenanthrene	25.02	178	1173	N.D.		
56) Anthracene	25.02	178	1173	N.D.		
57) Di-n-butylphthalate	27.02	149	4785	N.D.		
58) Fluoranthene	0.00	202	0	N.D.		
60) 3,3'-Dichlorobenzidine	0.00	252	0	N.D.		
61) Benzidine	0.00	184	0	N.D.		
63) Pyrene	0.00	202	0	N.D.		
64) Butylbenzylphthalate	31.54	149	869	N.D.		
65) Benzo(a)anthracene	33.06	228	4568	N.D.		
66) Bis(2-ethylhexyl)phthalate	33.33	149	4540	N.D.		
67) Chrysene	33.06	228	4568	N.D.		
69) Di-n-Octylphthalate	0.00	149	0	N.D.		
70) Benzo(b)fluoranthene	0.00	252	0	N.D.		

(#)=qualifier out of range (m)=manual integration

25048.D NP103001.M Mon Nov 19 15:04:08 2001

Page 2

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV0801\25048.D

Vial: 7

Acq On : 8 Nov 2001 8:28 pm

Operator: 209 GALOS

Sample : gc/ms unknown

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Nov 8 21:17 2001

Quant Results File: NP103001.RES

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Nov 02 16:41:16 2001

Response via : Initial Calibration

DataAcq Meth : NP103001

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
71) Benzo(k)fluoranthene	0.00	252	0	N.D.		
72) Benzo(a)pyrene	37.15	252	5688	N.D.		
73) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
74) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
75) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

 (#) = qualifier out of range (m) = manual integration
 25048.D NP103001.M Mon Nov 19 15:04:09 2001


Quantitation Report

Data File : C:\HPCHEM\1\DATA\NOV0801\25048.D
Acq On : 8 Nov 2001 8:28 pm
Sample : gc/ms unknown
Misc :
MS Integration Params: RTEINT.P
Quant Time: Nov 8 21:17 2001

Vial: 7
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: NP103001.RES

Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Fri Nov 02 16:41:16 2001
Response via : Initial Calibration

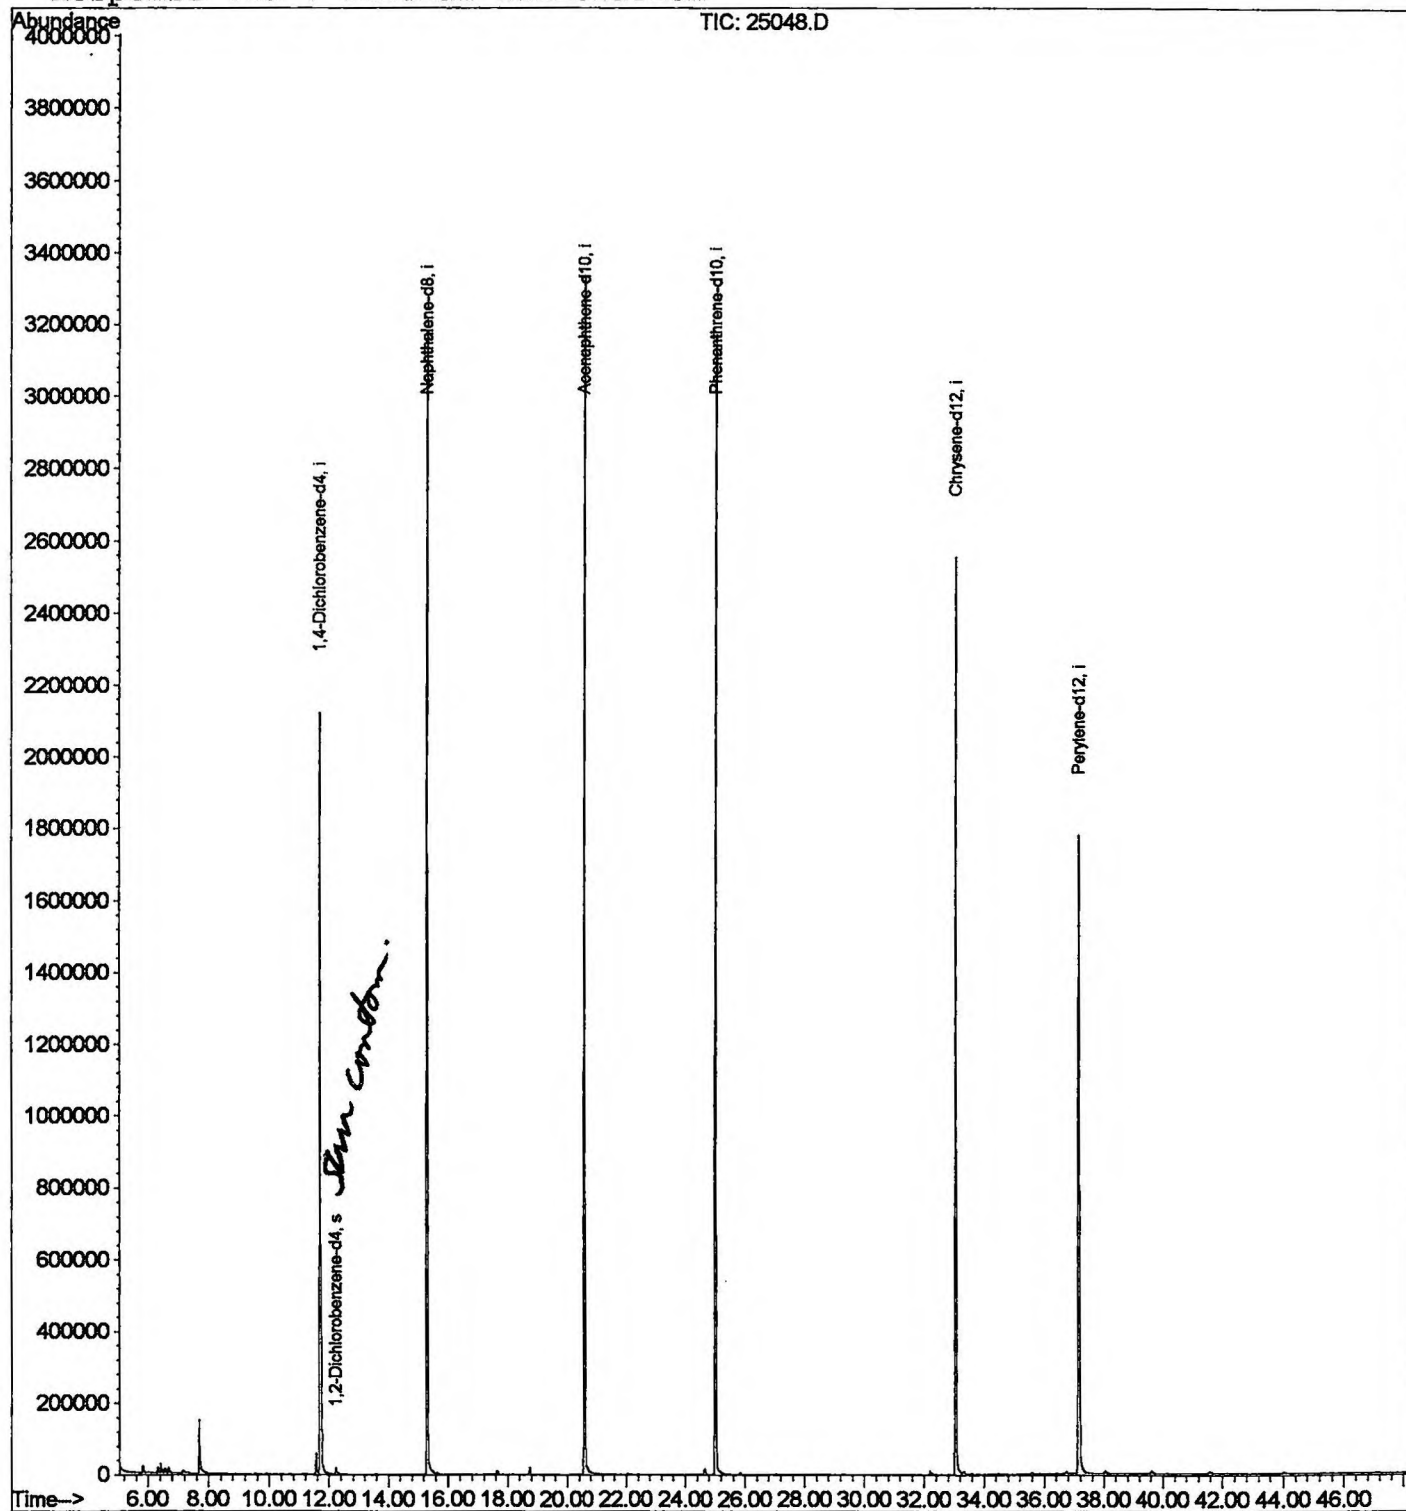

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\NOV0801\25048.D
 Acq On : 8 Nov 2001 8:28 pm
 Sample : gc/ms unknown
 Misc :
 MS Integration Params: LSCINT.P

Vial: 7
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC




peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	7.694	285	289	311	rBV	151176	400383	5.19%	1.029%
2	11.568	707	711	721	rBV	58687	136161	1.77%	0.350%
3	11.706	721	726	747	rVV	2120642	5090795	66.01%	13.088%
4	15.314	1113	1119	1139	rBV	3181336	7050385	91.42%	18.126%
5	20.602	1688	1695	1712	rBV	3335456	7712356	100.00%	19.828%
6	25.027	2170	2177	2190	rBV2	3168909	7260882	94.15%	18.667%
7	33.059	3044	3052	3074	rBV2	2553203	5987312	77.63%	15.393%
8	37.163	3489	3499	3523	rBV2	1777149	5257694	68.17%	13.517%

Sum of corrected areas: 38895968

25048.D NP103001.M Mon Nov 19 15:09:00 2001

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\NOV0801\25048.D
 Operator : 209 GALOS
 Acquired : 8 Nov 2001 8:28 pm using AcqMethod NP103001
 Instrument : GC/MS 209
 Sample Name: gc/ms unknown
 Misc Info :
 Vial Number: 7
 Quant File :NP103001.RES (RTE Integrator)

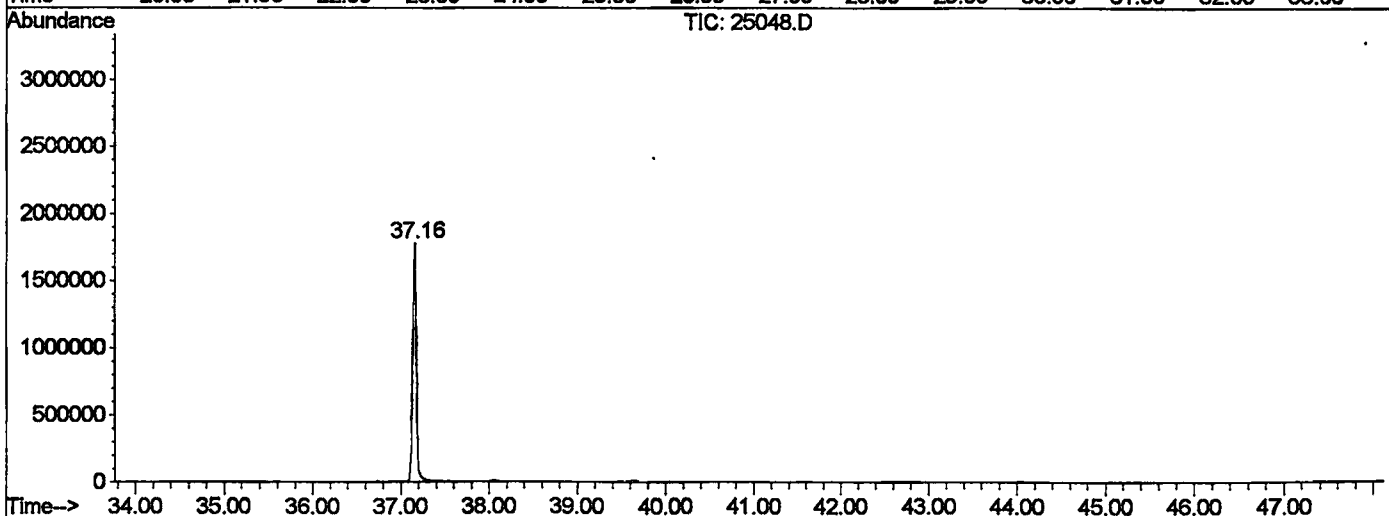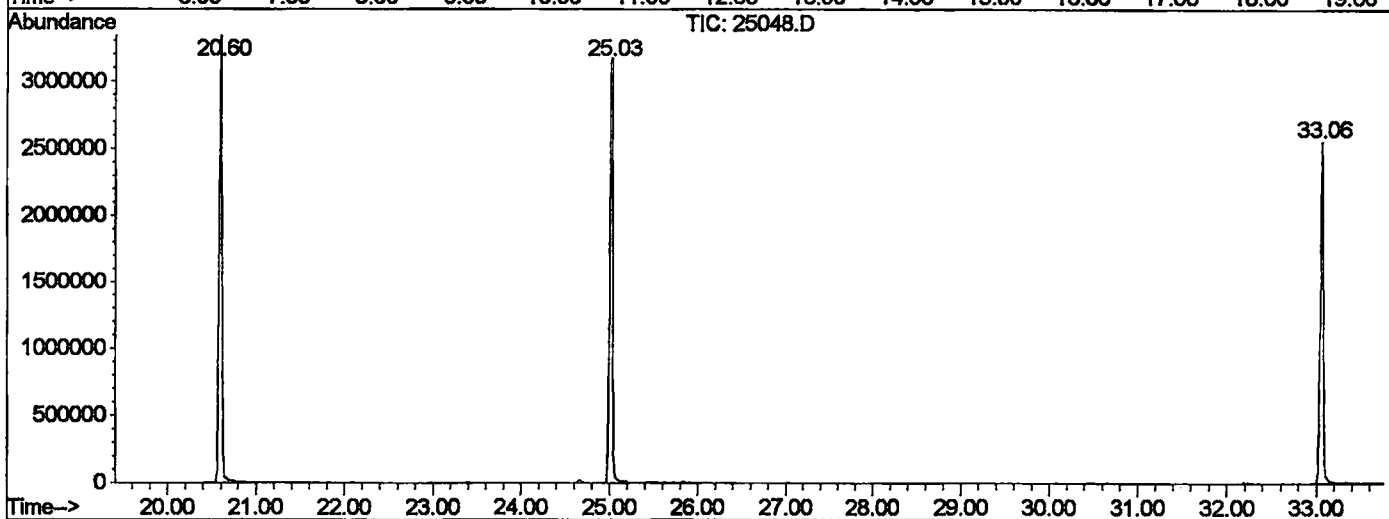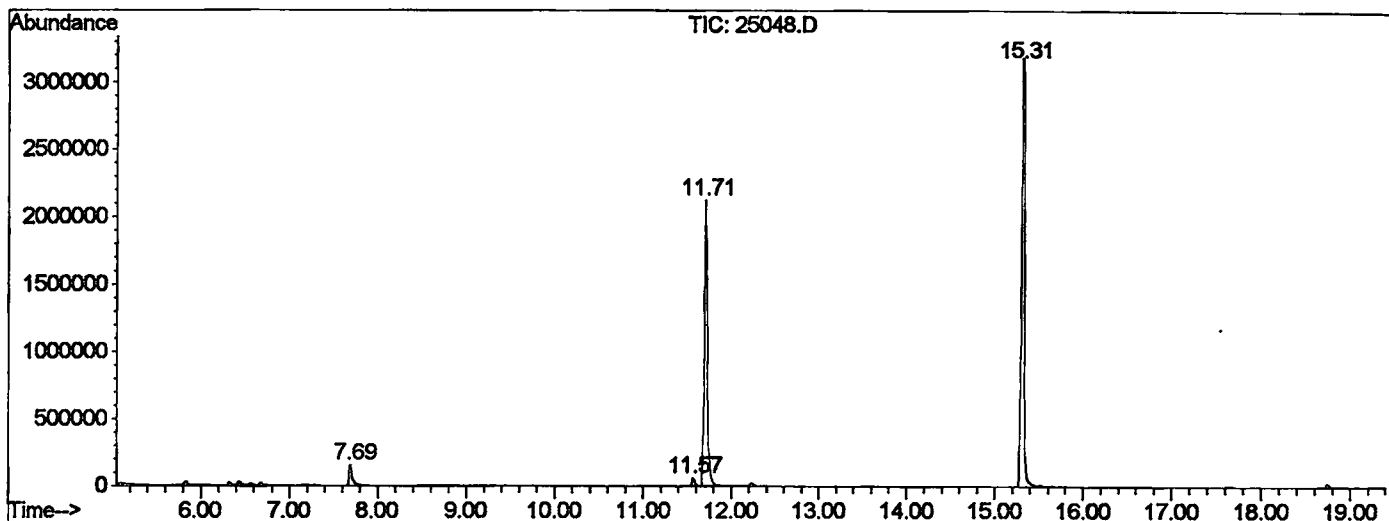

25048.D NP103001.M Mon Nov 19 15:09:03 2001

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\NOV0801\25048.D
Acq On : 8 Nov 2001 8:28 pm
Sample : gc/ms unknown
Misc :
MS Integration Params: LSCINT.P


Vial: 7
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.69	1.57 ug/l	400383	1,4-Dichlorobenzene-d4	11.71

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	38
2			3-Hydroxy-2-pentanone	102	C5H10O2	003142-66-3	9
3			Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9
4			Acetic acid, 1,1-dimethylethyl este	116	C6H12O2	000540-88-5	9

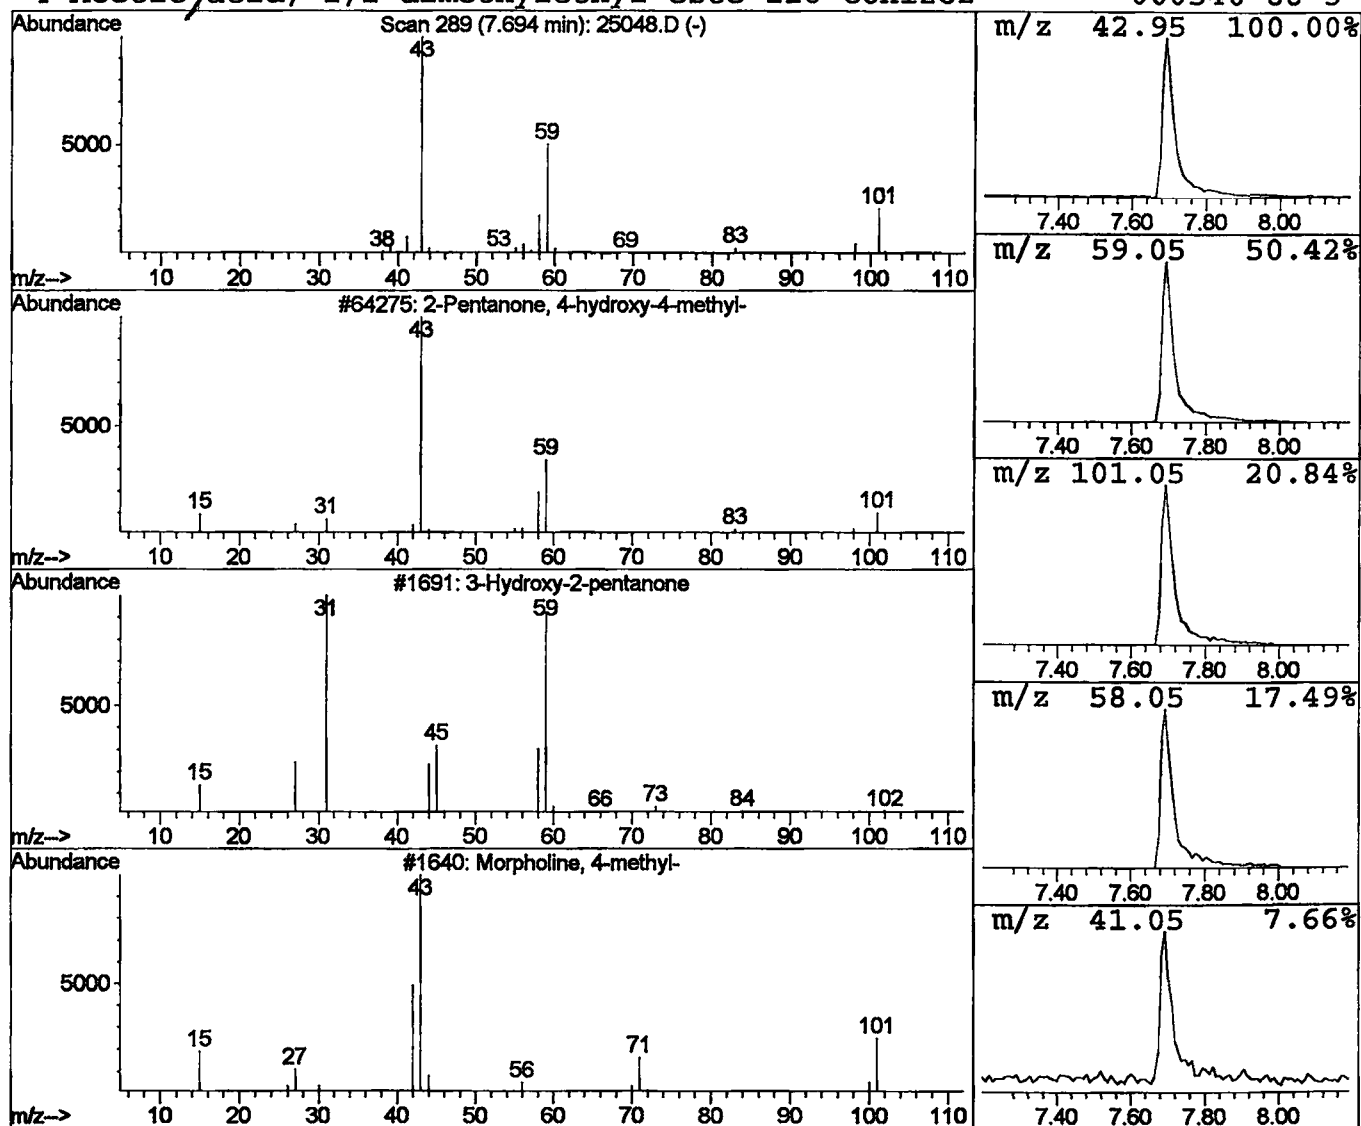

Library Search Compound Report


Data File : C:\HPCHEM\1\DATA\NOV0801\25048.D
Acq On : 8 Nov 2001 8:28 pm
Sample : gc/ms unknown
Misc :
MS Integration Params: LSCINT.P

Vial: 7
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 2 1,4-Dichlorobenzene-d4 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.	
11.57	0.53 ug/l	136161	1,4-Dichlorobenzene-d4	11.71	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	1,4-Dichlorobenzene-d4	150	C6Cl2D4	003855-82-1	64
2	Benzene-1,2,3,4-d4-, 5,6-dichloro-	150	C6Cl2D4	002199-69-1	38
3	Acenaphthylene	152	C12H8	000208-96-8	10
4	Biphenylene	152	C12H8	000259-79-0	9

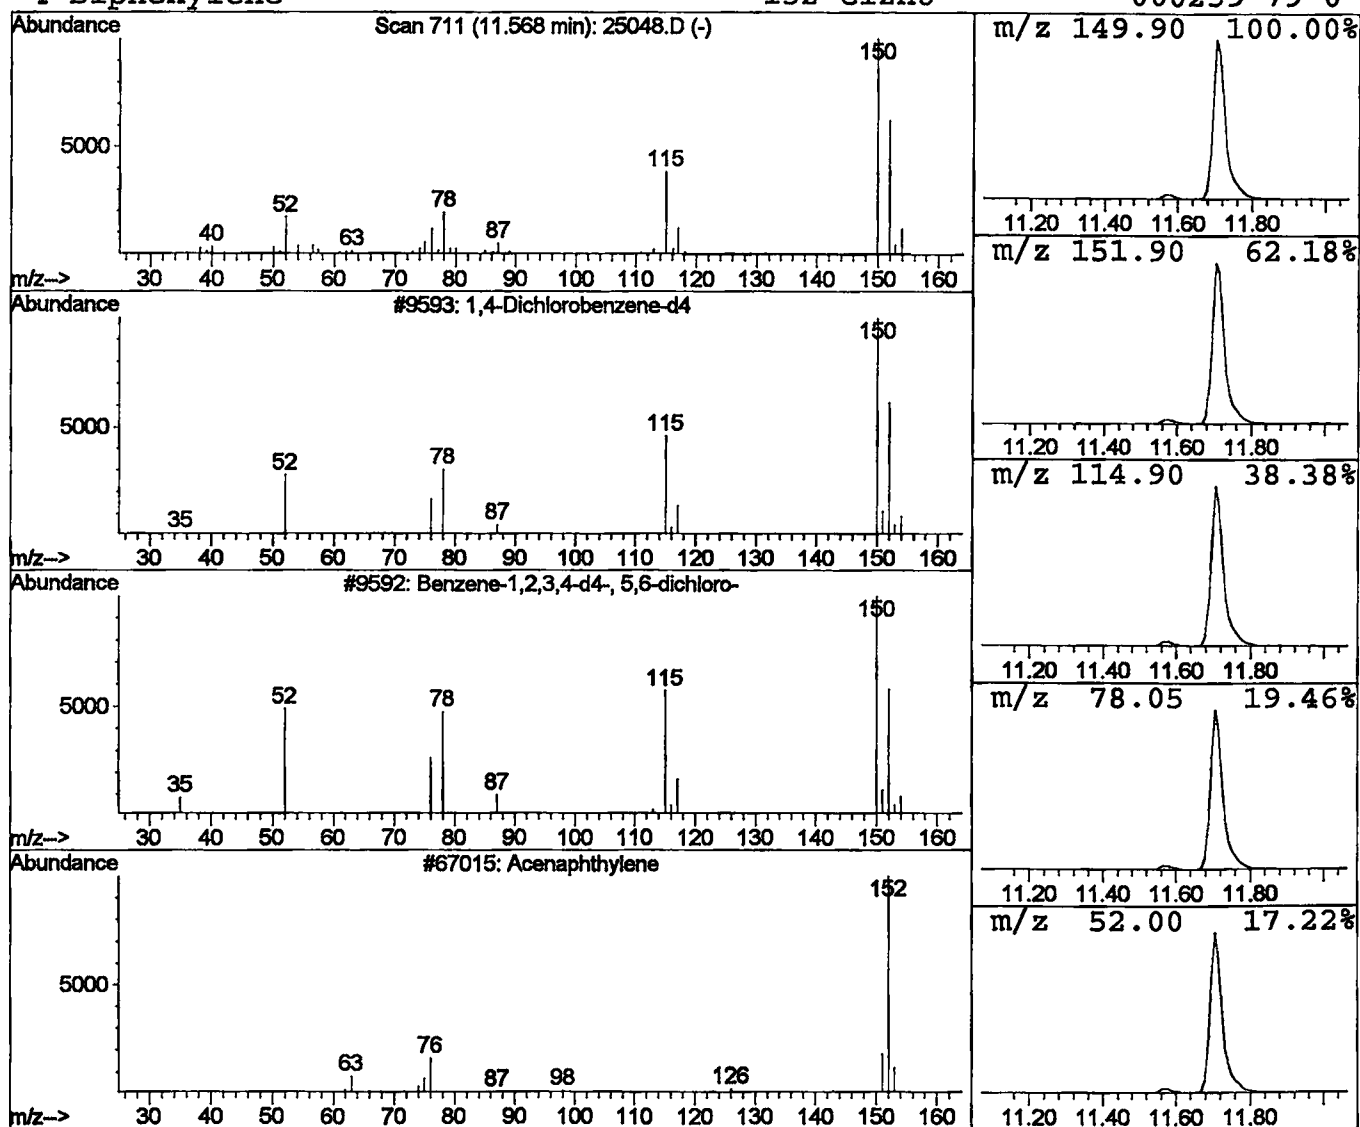

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 8 Nov 2001 8:28 pm
 Data File: C:\HPCHEM\1\DATA\NOV0801\25048.D
 Name: gc/ms unknown
 Misc:
 Method: C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	7.69	1.6	ug/l	400383	ISTD01	11.71	5090800	20.0
1,4-Dichlorobenzene-	11.57	0.5	ug/l	136161	ISTD01	11.71	5090800	20.0

25048.D NP103001.M Mon Nov 19 15:09:09 2001