

Method

508

bumb

Date Extracted

10/23/01

Page

45

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count
	LB	500ml		1ml			2ml		27	
	Ref test				1ml					
	MDL test				1ml					
	PRL 1260				1ml					
✓	25049									9
✓	25050									10
✓	25051									11
✓	25052									12
✓	25072									13
✓	25073									14
✓	25154									15
✓	25155									16
✓	25259									17
✓	25260									18
✓	25261									19
✓	25262									20
✓	25263									21
Remarks										
Reviewed by, <u>[Signature]</u> 11/1/01										
drip rate must be between 5-15 ml/min for liq-liq extractors drip rate -										
Extraction type - <u>SDFunne</u>		Solv. lot# <u>V29E108</u>		NaCl lot# <u>V1549</u>		Na2SO4 lot# <u>V32603</u>				
STANDARD	INT STD LOG#									
CALIBRATION										
REF/SPIKE	<u>2062a</u>	<u>PRL1260 - 7/13/01</u>								
MDL/MDRF	<u>2062a</u>									
Q. CHECK										
INT. STD.										
SURROGATE	<u>2064c</u>									
LPC										
ENDRIN/DDT										

Analyst

C.N./AD

revision 4/12/01

Verified by

Reviewed by

Date

[Signature]
11/29/01

Sequence Name: C:\HPCHEM\1\SEQUENCE\NOV0901.S

Comment: INST 209; 30Mx0.25umX0.50

Operator: 209 GALOS

Data Path: C:\HPCHEM\1\data\nov0901\

Pre-Seq Cmd:

Post-Seq Cmd:


Method Sections To Run	On A Barcode Mismatch
(X) Full Method	(X) Inject Anyway
() Reprocessing Only	() Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	NP103001	
2	Sample	2	LB	NP103001	10/23
3	Sample	3	25155	NP103001	gc/ms unknown
4	Sample	4	25263	NP103001	gc/ms unknown
5	Sample	5	25049	NP103001	gc/ms unknown
6	Sample	6	25050	NP103001	gc/ms unknown
7	Sample	7	25051	NP103001	gc/ms unknown
8	Sample	8	25259	NP103001	gc/ms unknown
9	Sample	9	25154	NP103001	gc/ms unknown
10	Sample	10	25260	NP103001	gc/ms unknown
11	Sample	11	25261	NP103001	gc/ms unknown
12	Sample	12	25262	NP103001	gc/ms unknown
13	Sample	13	25072	NP103001	gc/ms unknown
14	Sample	14	25073	NP103001	gc/ms unknown
15	Sample	15	25052	NP103001	gc/ms unknown
16	Sample	16	LBB	NP103001	lb blk 10/23
17	Sample	17	25174	NP103001	gc/ms unknown
18	Sample	18	25175	NP103001	gc/ms unknown
19	Sample	19	25045	NP103001	gc/ms unknown
20	Sample	20	25178	NP103001	gc/ms unknown

DFTPP

Data File : C:\HPCHEM\1\DATA\NOV0901\DFTPP.D
 Acq On : 9 Nov 2001 11:27 am
 Sample :
 Misc :
 MS Integration Params: RTEINT.P
 Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

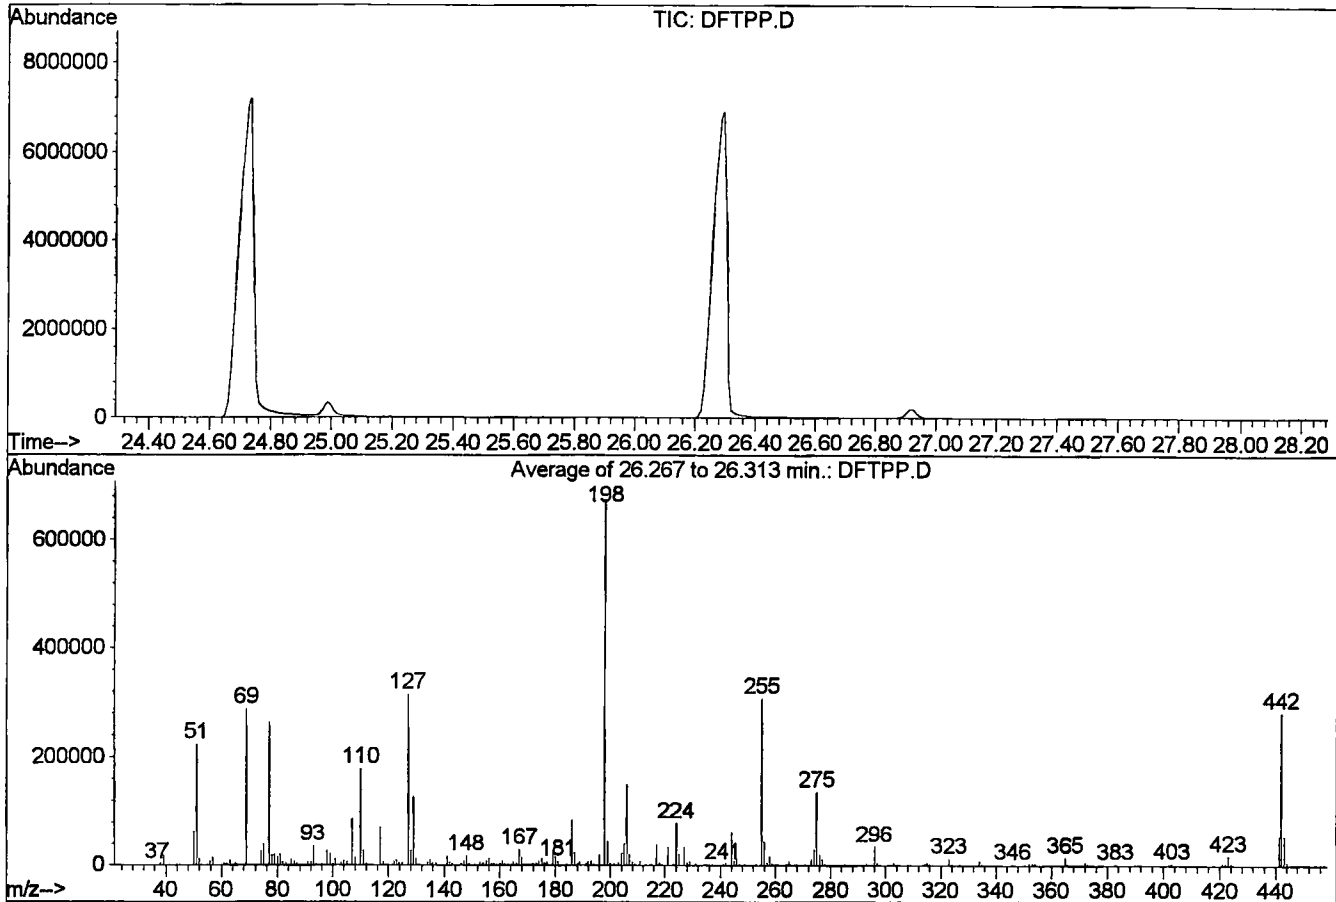

Spectrum Information: Average of 26.267 to 26.313 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	33.1	223091	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.7	287664	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	46.9	315453	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	673136	PASS
199	198	5	9	6.6	44325	PASS
275	198	10	30	20.2	136083	PASS
365	198	1	100	2.0	13271	PASS
441	443	0.01	100	97.4	52448	PASS
442	198	40	110	41.9	282336	PASS
443	442	17	23	19.1	53847	PASS