

User: Galos, Marie
Westchester Dept. of Labs & Research
Date: 11/28/2001 Time: 10:00:23

Sample: AD25072
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 11/28/01 09:59 Ended: 11/28/01 09:59 Analyst: MG
Page: 1

	Component Name	Vol	Result
1	Other unknown compounds		see comment

Comments for Sample AD25072 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Galos, Marie

Date: 11-28-2001 Time: 10:00:30

A scan of the extract prepared for the 508 analysis, from 35-550 amu using a mass spectrometer, does not reveal the presence of non-target compounds.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV0901\25072.D
 Acq On : 10 Nov 2001 12:07 am
 Sample : gc/ms unknown
 Misc :
 MS Integration Params: RTEINT.P
 Quant Time: Nov 10 0:56 2001

Vial: 13
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: NP103001.RES

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Fri Nov 02 16:41:16 2001
 Response via : Initial Calibration
 DataAcq Meth : NP103001

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	11.71	152	552870	20.00	ug/l	-0.01
19) Naphthalene-d8	15.32	136	2104129	20.00	ug/l	-0.01
31) Acenaphthene-d10	20.60	164	1053467	20.00	ug/l	-0.01
49) Phenanthrene-d10	25.01	188	1546372	20.00	ug/l	-0.02
59) Chrysene-d12	33.06	240	1089112	20.00	ug/l	-0.01
68) Perylene-d12	37.15	264	809992	20.00	ug/l	-0.01

System Monitoring Compounds

4) 2-Fluorophenol	0.00	112	0	0.00	ug/l	
Spiked Amount	75.000		Recovery	=	0.00%	
5) Phenol-d5	0.00	99	0	0.00	ug/l	
Spiked Amount	75.000		Recovery	=	0.00%	
6) 2-Chlorophenol-d4	11.70	132	338	0.01	ug/l	0.46
Spiked Amount	75.000		Recovery	=	0.01%	
7) 1,2-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	
Spiked Amount	50.000		Recovery	=	0.00%	
20) Nitrobenzene-d5	0.00	82	0	0.00	ug/l	
Spiked Amount	50.000		Recovery	=	0.00%	
32) 2-Fluorobiphenyl	18.75	172	1128	0.02	ug/l	0.13
Spiked Amount	50.000		Recovery	=	0.04%	
33) 2,4,6-Tribromophenol	0.00	330	0	0.00	ug/l	
Spiked Amount	75.000		Recovery	=	0.00%	
62) Terphenyl-d14	0.00	244	0	0.00	ug/l	
Spiked Amount	50.000		Recovery	=	0.00%	

Target Compounds

					Qvalue
2) Pyridine	0.00	79	0	N.D.	
3) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
8) Phenol	0.00	94	0	N.D.	
9) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
10) 2-Chlorophenol	0.00	128	0	N.D.	
11) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
12) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
13) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
14) 2-Methylphenol	0.00	108	0	N.D.	
15) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
16) 3&4-Methylphenol	0.00	108	0	N.D.	
17) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
18) Hexachloroethane	0.00	117	0	N.D.	
21) Nitrobenzene	0.00	77	0	N.D.	
22) Isophorone	0.00	82	0	N.D.	

(#) = qualifier out of range (m) = manual integration

25072.D GCMS1126.M Tue Nov 27 14:39:37 2001

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV0901\25072.D

Vial: 13

Acq On : 10 Nov 2001 12:07 am

Operator: 209 GALOS

Sample : gc/ms unknown

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Nov 10 0:56 2001

Quant Results File: NP103001.RES

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Nov 02 16:41:16 2001

Response via : Initial Calibration

DataAcq Meth : NP103001

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
23) 2-Nitrophenol	0.00	139	0	N.D.		
24) 2,4-Dimethylphenol	0.00	107	0	N.D.		
25) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.		
26) 2,4-Dichlorophenol	0.00	162	0	N.D.		
27) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.		
28) Naphthalene	15.38	128	345	N.D.		
29) Hexachlorobutadiene	0.00	225	0	N.D.		
30) 4-Chloro-3-methylphenol	0.00	107	0	N.D.		
34) Hexachlorocyclopentadiene	0.00	237	0	N.D.		
35) 2,4,6-Trichlorophenol	0.00	196	0	N.D.		
36) 2,4,5-Trichlorophenol	0.00	196	0	N.D.		
37) 2-Chloronaphthalene	0.00	162	0	N.D.		
38) Dimethylphthalate	0.00	163	0	N.D.		
39) 2,6-Dinitrotoluene	0.00	165	0	N.D.		
40) Acenaphthylene	0.00	152	0	N.D.		
41) Acenaphthene	0.00	153	0	N.D.		
42) 2,4-Dinitrophenol	0.00	184	0	N.D.		
43) 4-Nitrophenol	0.00	65	0	N.D.		
44) 2,4-Dinitrotoluene	20.88	165	595	N.D.		
45) Diethylphthalate	0.00	149	0	N.D.		
46) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.		
47) Fluorene	0.00	166	0	N.D.		
48) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.		
50) 4,6-Dinitro-2-methylphenol	0.00	198	0	N.D.		
51) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
52) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
53) Hexachlorobenzene	0.00	284	0	N.D.		
54) Pentachlorophenol	0.00	266	0	N.D.		
55) Phenanthrene	25.02	178	621	N.D.		
56) Anthracene	25.02	178	621	N.D.		
57) Di-n-butylphthalate	27.02	149	1804	N.D.		
58) Fluoranthene	0.00	202	0	N.D.		
60) 3,3'-Dichlorobenzidine	0.00	252	0	N.D.		
61) Benzidine	0.00	184	0	N.D.		
63) Pyrene	0.00	202	0	N.D.		
64) Butylbenzylphthalate	0.00	149	0	N.D.		
65) Benzo(a)anthracene	33.06	228	2770	N.D.		
66) Bis(2-ethylhexyl)phthalate	33.33	149	571	N.D.		
67) Chrysene	33.06	228	2770	N.D.		
69) Di-n-Octylphthalate	0.00	149	0	N.D.		
70) Benzo(b)fluoranthene	0.00	252	0	N.D.		

(#) = qualifier out of range (m) = manual integration

25072.D GCMS1126.M Tue Nov 27 14:39:42 2001

Page 2

Quantitation Report (QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV0901\25072.D

Vial: 13

Acq On : 10 Nov 2001 12:07 am

Operator: 209 GALOS

Sample : gc/ms unknown

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Nov 10 0:56 2001

Quant Results File: NP103001.RES

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Nov 02 16:41:16 2001

Response via : Initial Calibration

DataAcq Meth : NP103001

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
71) Benzo(k)fluoranthene	0.00	252	0	N.D.		
72) Benzo(a)pyrene	37.16	252	3132	N.D.		
73) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
74) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
75) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

25072.D GCMS1126.M Tue Nov 27 14:39:43 2001

Page 3


Quantitation Report

Data File : C:\HPCHEM\1\DATA\NOV0901\25072.D
Acq On : 10 Nov 2001 12:07 am
Sample : gc/ms unknown
Misc :
MS Integration Params: RTEINT.P
Quant Time: Nov 10 0:56 2001

Vial: 13
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: NP103001.RES

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Tue Nov 27 12:20:14 2001
Response via : Initial Calibration

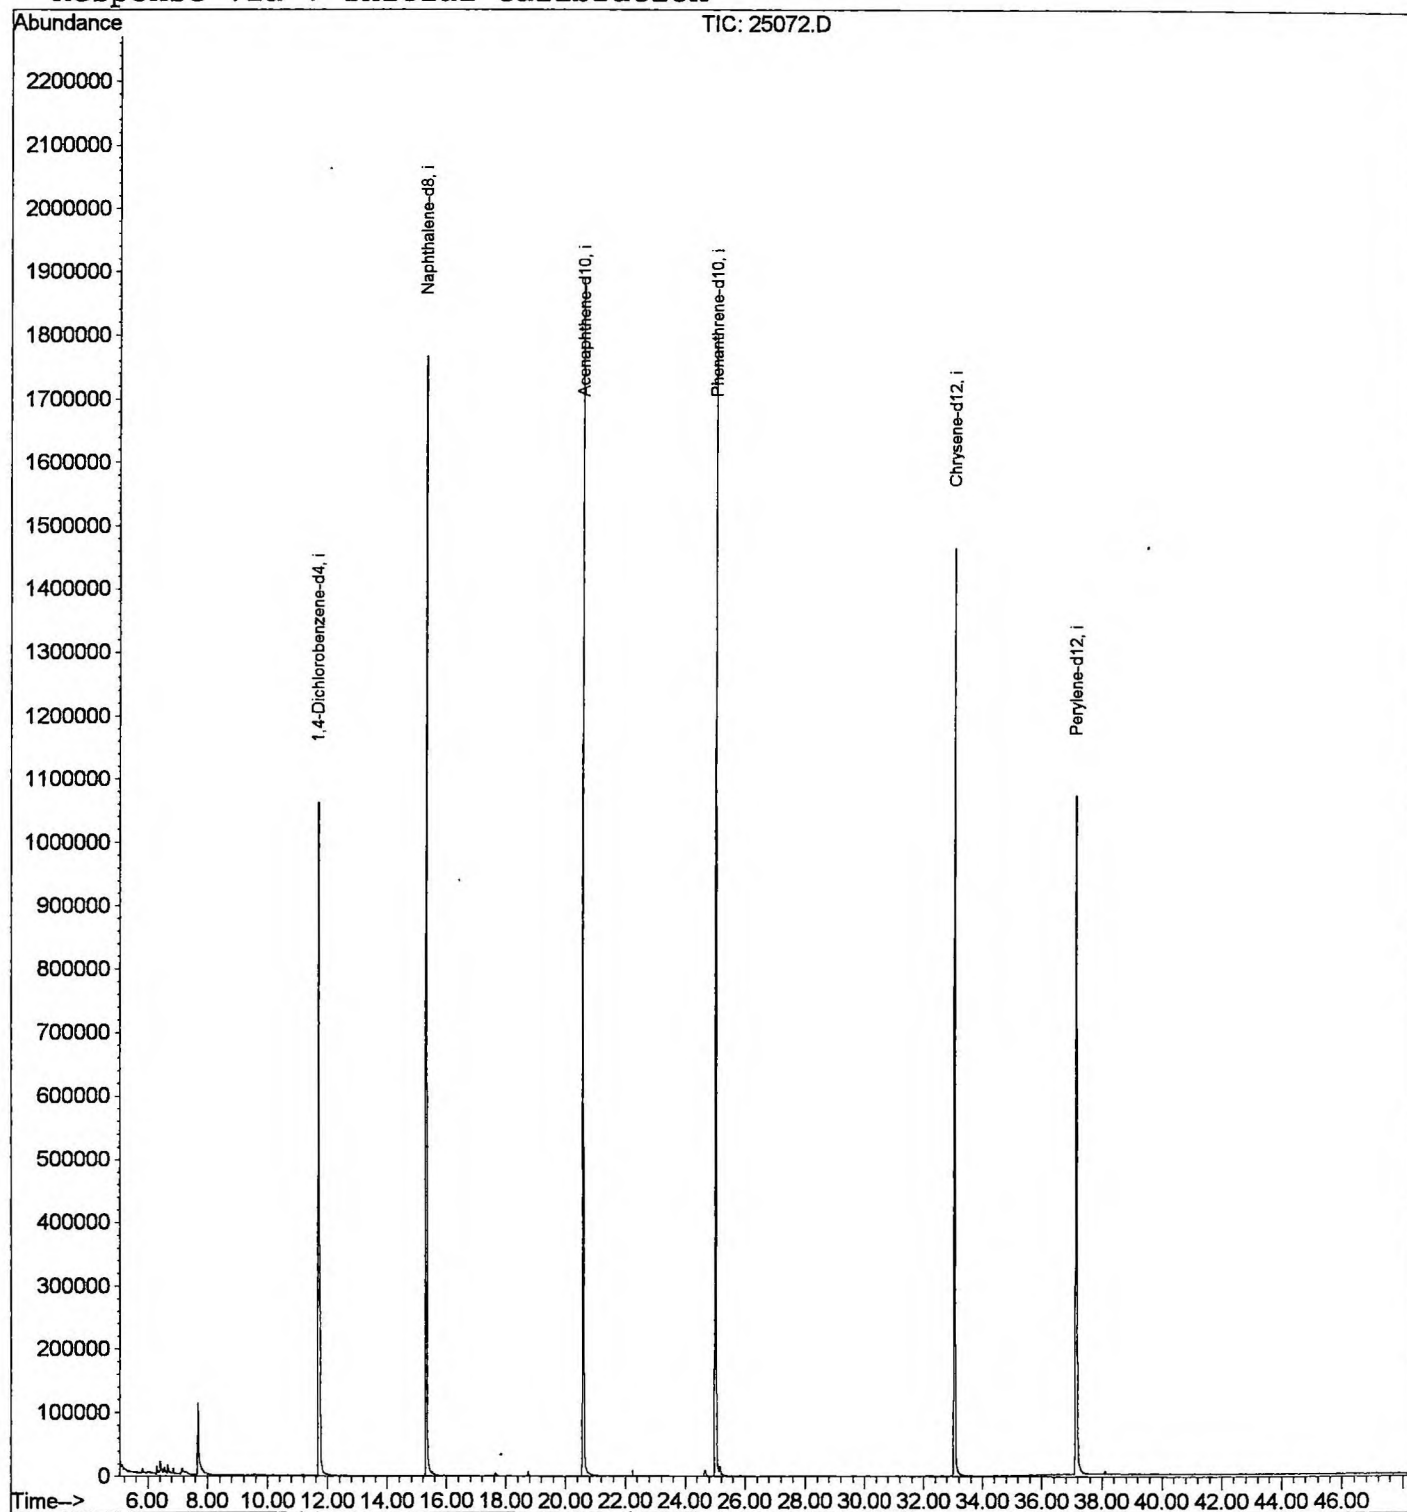

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\NOV0901\25072.D

Acq On : 10 Nov 2001 12:07 am

Sample : gc/ms unknown

Misc :

MS Integration Params: LSCINT.P

Vial: 13

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	6.423	147	150	161	rVV	18485	50977	1.21%	0.234%
2	7.681	284	287	314	rBV	111710	344355	8.19%	1.578%
3	11.711	721	726	747	rBV	1061960	2864063	68.11%	13.128%
4	15.319	1113	1119	1136	rBV	1766580	3832373	91.14%	17.567%
5	20.598	1687	1694	1709	rBV	1891493	4204805	100.00%	19.274%
6	25.013	2169	2175	2187	rBV2	1802201	3989511	94.88%	18.287%
7	25.160	2187	2191	2203	rVB3	14528	49496	1.18%	0.227%
8	33.055	3044	3051	3068	rBV2	1465575	3428240	81.53%	15.714%
9	37.150	3488	3497	3518	rBV2	1071727	3052006	72.58%	13.990%




Sum of corrected areas: 21815826

25072.D NP103001.M

Tue Nov 27 11:11:13 2001

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\NOV0901\25072.D
Operator : 209 GALOS
Acquired : 10 Nov 2001 12:07 am using AcqMethod NP103001
Instrument : GC/MS 209
Sample Name: gc/ms unknown
Misc Info :
Vial Number: 13
Quant File :NP103001.RES (RTE Integrator)

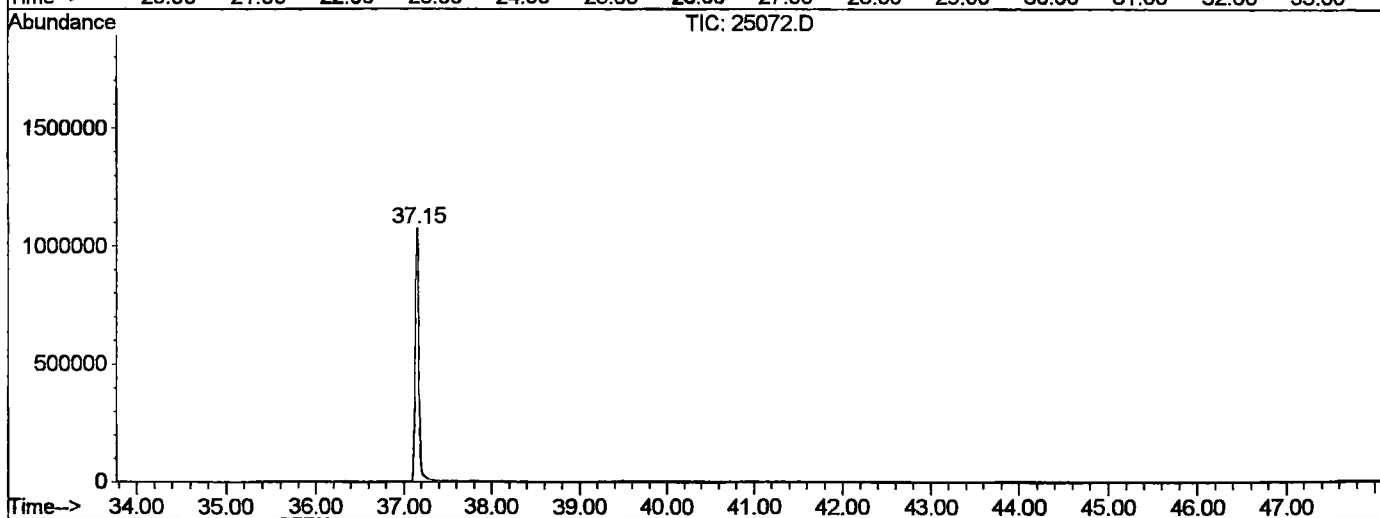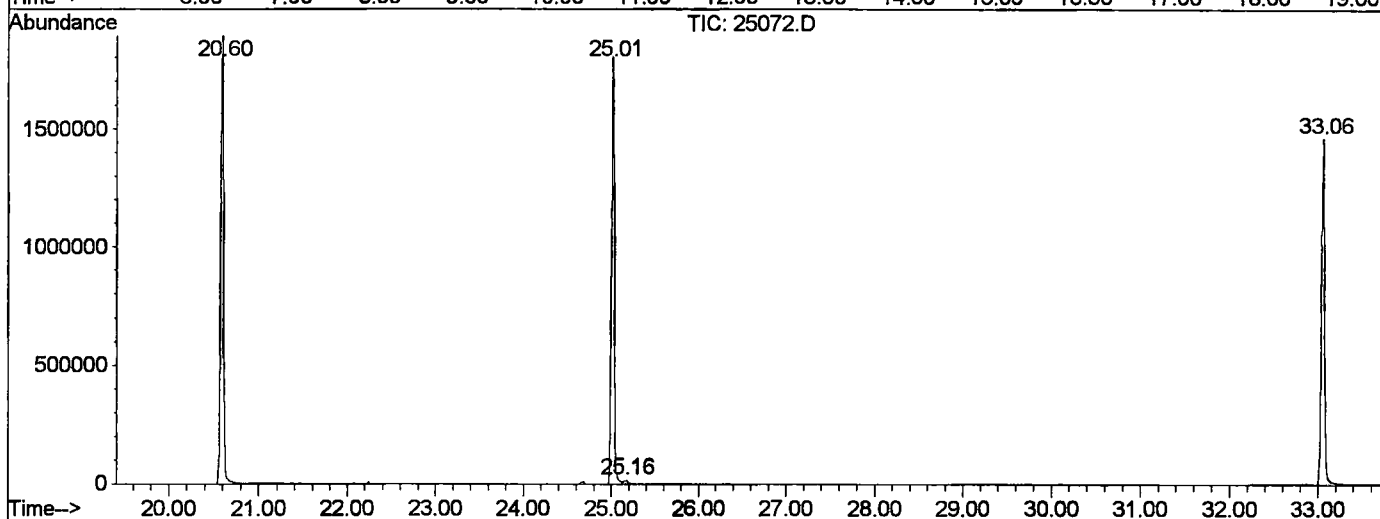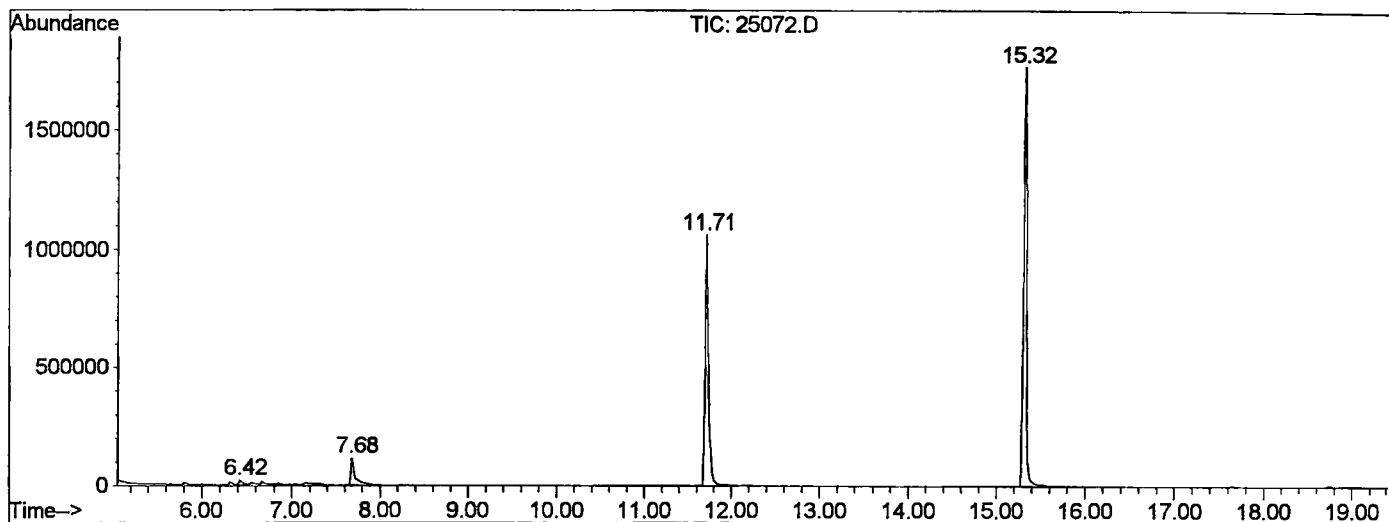

25072.D NP103001.M Tue Nov 27 11:11:15 2001

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\NOV0901\25072.D
 Acq On : 10 Nov 2001 12:07 am
 Sample : gc/ms unknown
 Misc :
 MS Integration Params: LSCINT.P


Vial: 13
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.68	2.40 ug/l	344355	1,4-Dichlorobenzene-d4	11.71

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50
2		2-Propanol, 2-methyl-	74	C4H10O	000075-65-0	17
3		Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9
4		3-Hydroxy-2-pentanone	102	C5H10O2	003142-66-3	9

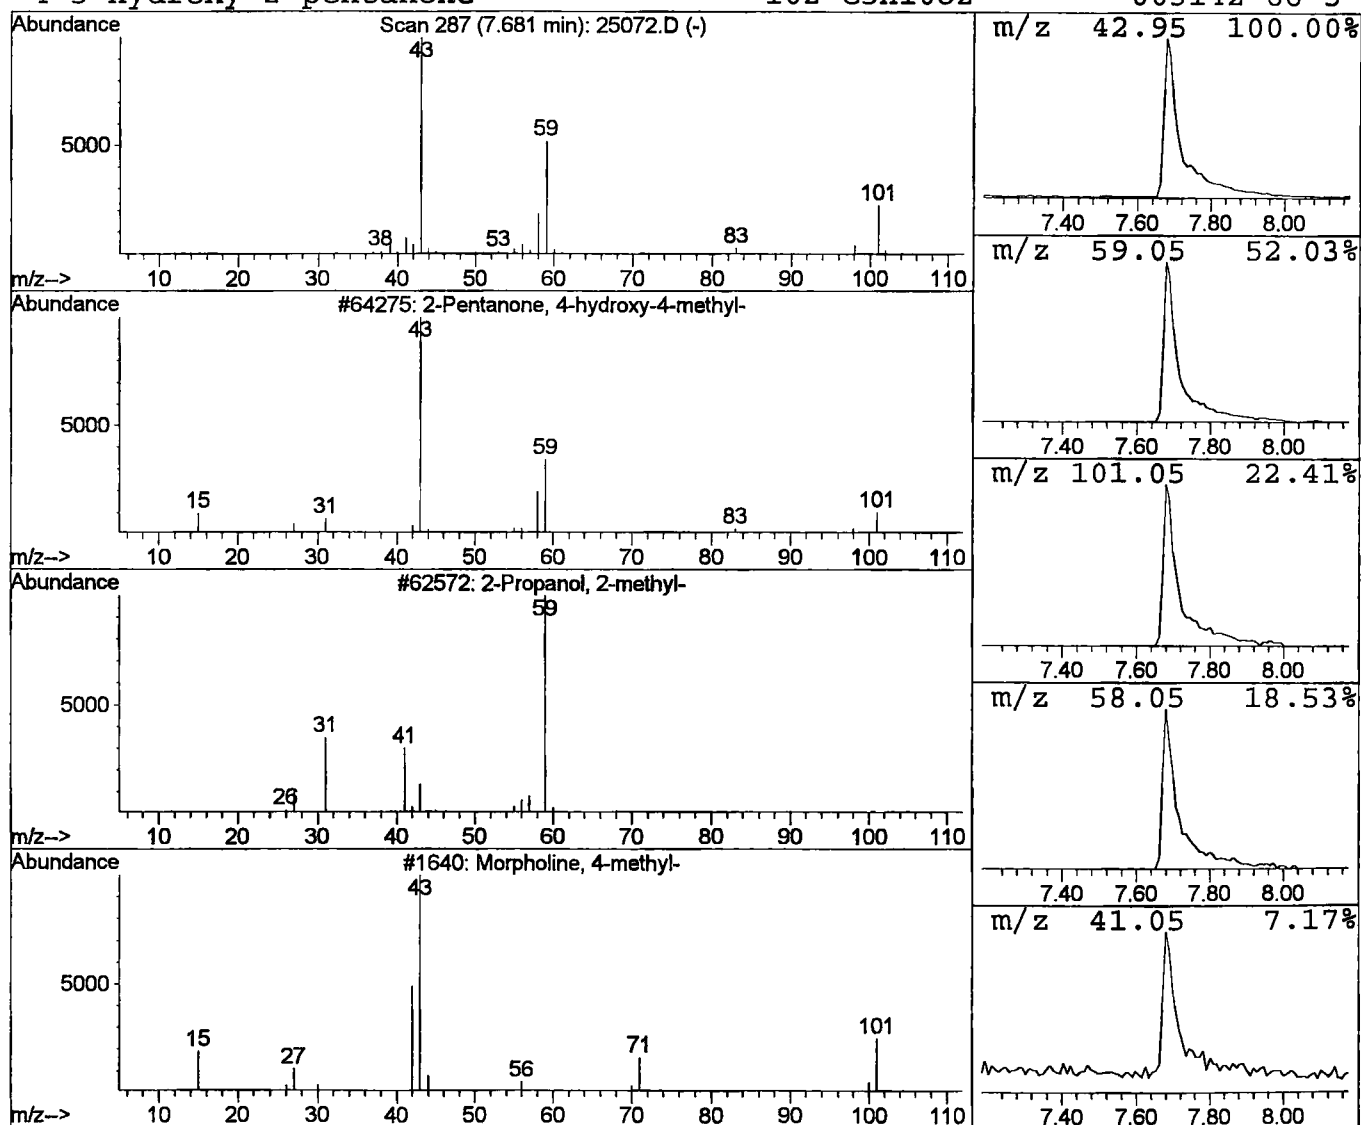

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 10 Nov 2001 12:07 am
Data File: C:\HPCHEM\1\DATA\NOV0901\25072.D
Name: gc/ms unknown
Misc:
Method: C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	7.68	2.4	ug/l	344355	ISTD01	11.71	2864060	20.0

25072.D NP103001.M Tue Nov 27 11:11:20 2001