User: Galos, Marie
Westchester Dept. of Labs & Research
Date: 11/28/2001 Time: 09:50:07

Sample: AD25260
Analysis: $GCMS GCMS Scan For Unknowns
Units: ug
Started: 11/28/01 09:49 Ended: 11/28/01 09:49 Analyst: MG
Page: 1

	Component Name	Viol	Result
1	Other unknown compounds		see comment

Comments for Sample AD25260 - Analysis $GCMS

Westchester Dept. of Labs & Research
User: Galos, Marie
Date: 11-28-2001 Time: 09:50:19

A scan of the extract prepared for the 508 analysis, from 35-550 amu using a mass spectrometer, does not reveal the presence of non-target compounds.

Quantitation Report (QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV0901\25260.D Vial: 10
Acq On : 9 Nov 2001 9:13 pm Operator: 209 GALOS
Sample : gc/ms unknown Inst : GC/MS 209
Misc : Multiplr: 1.00
MS Integration Params: RTEINT.P
Quant Time: Nov 9 22:01 2001 Quant Results File: NP103001.RES

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Fri Nov 02 16:41:16 2001
Response via : Initial Calibration
DataAcq Meth : NP103001

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	11.71	152	643492	20.00	ug/l	-0.02
19) Naphthalene-d8	15.32	136	2477876	20.00	ug/l	-0.02
31) Acenaphthene-d10	20.59	164	1269468	20.00	ug/l	-0.02
49) Phenanthrene-d10	25.02	188	1858632	20.00	ug/l	-0.02
59) Chrysene-d12	33.05	240	1234759	20.00	ug/l	-0.02
68) Perylene-d12	37.16	264	892756	20.00	ug/l	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	0.00	112	0	0.00	ug/l	
Spiked Amount 75.000			Recovery =	0.00%		
5) Phenol-d5	0.00	99	0	0.00	ug/l	
Spiked Amount 75.000			Recovery =	0.00%		
6) 2-Chlorophenol-d4	11.71	132	429	0.01	ug/l	0.47
Spiked Amount 75.000			Recovery =	0.01%		
7) 1,2-Dichlorobenzene-d4	12.26	152	309	0.01	ug/l	0.01
Spiked Amount 50.000			Recovery =	0.02%		
20) Nitrobenzene-d5	0.00	82	0	0.00	ug/l	
Spiked Amount 50.000			Recovery =	0.00%		
32) 2-Fluorobiphenyl	18.75	172	1683	0.02	ug/l	0.13
Spiked Amount 50.000			Recovery =	0.04%		
33) 2,4,6-Tribromophenol	0.00	330	0	0.00	ug/l	
Spiked Amount 75.000			Recovery =	0.00%		
62) Terphenyl-d14	0.00	244	0	0.00	ug/l	
Spiked Amount 50.000			Recovery =	0.00%		
Target Compounds						Qvalue
2) Pyridine	0.00	79	0	N.D.		
3) N-nitroso-dimethyl amine	0.00	74	0	N.D.		
8) Phenol	0.00	94	0	N.D.		
9) bis(2-Chloroethyl)ether	0.00	93	0	N.D.		
10) 2-Chlorophenol	0.00	128	0	N.D.		
11) 1,3-Dichlorobenzene	0.00	146	0	N.D.		
12) 1,4-Dichlorobenzene	0.00	146	0	N.D.		
13) 1,2-Dichlorobenzene	0.00	146	0	N.D.		
14) 2-Methylphenol	0.00	108	0	N.D.		
15) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.		
16) 3&4-Methylphenol	0.00	108	0	N.D.		
17) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.		
18) Hexachloroethane	0.00	117	0	N.D.		
21) Nitrobenzene	0.00	77	0	N.D.		
22) Isophorone	0.00	82	0	N.D.		

(#) = qualifier out of range (m) = manual integration

Quantitation Report (QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV0901\25260.D Vial: 10
Acq On : 9 Nov 2001 9:13 pm Operator: 209 GALOS
Sample : gc/ms unknown Inst : GC/MS 209
Misc : Multiplr: 1.00
MS Integration Params: RTEINT.P
Quant Time: Nov 9 22:01 2001 Quant Results File: NP103001.RES

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Fri Nov 02 16:41:16 2001
Response via : Initial Calibration
DataAcq Meth : NP103001

	Compound	R.T.	QIon	Response	Conc Unit	Qvalue
23)	2-Nitrophenol	0.00	139	0	N.D.	
24)	2,4-Dimethylphenol	0.00	107	0	N.D.	
25)	bis(2-Chloroethoxy)methane	0.00	93	0	N.D.	
26)	2,4-Dichlorophenol	0.00	162	0	N.D.	
27)	1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
28)	Naphthalene	0.00	128	0	N.D.	
29)	Hexachlorobutadiene	0.00	225	0	N.D.	
30)	4-Chloro-3-methylphenol	0.00	107	0	N.D.	
34)	Hexachlorocyclopentadiene	0.00	237	0	N.D.	
35)	2,4,6-Trichlorophenol	0.00	196	0	N.D.	
36)	2,4,5-Trichlorophenol	0.00	196	0	N.D.	
37)	2-Chloronaphthalene	0.00	162	0	N.D.	
38)	Dimethylphthalate	0.00	163	0	N.D.	
39)	2,6-Dinitrotoluene	0.00	165	0	N.D.	
40)	Acenaphthylene	0.00	152	0	N.D.	
41)	Acenaphthene	0.00	153	0	N.D.	
42)	2,4-Dinitrophenol	0.00	184	0	N.D.	
43)	4-Nitrophenol	0.00	65	0	N.D.	
44)	2,4-Dinitrotoluene	20.85	165	303	N.D.	
45)	Diethylphthalate	0.00	149	0	N.D.	
46)	4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
47)	Fluorene	0.00	166	0	N.D.	
48)	Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
50)	4,6-Dinitro-2-methylphenol	0.00	198	0	N.D.	
51)	N-Nitrosodiphenylamine	0.00	168	0	N.D.	
52)	4-Bromophenyl-phenylether	0.00	248	0	N.D.	
53)	Hexachlorobenzene	0.00	284	0	N.D.	
54)	Pentachlorophenol	0.00	266	0	N.D.	
55)	Phenanthrene	25.01	178	560	N.D.	
56)	Anthracene	25.01	178	560	N.D.	
57)	Di-n-butylphthalate	27.03	149	4325	N.D.	
58)	Fluoranthene	0.00	202	0	N.D.	
60)	3,3'-Dichlorobenzidine	0.00	252	0	N.D.	
61)	Benzidine	0.00	184	0	N.D.	
63)	Pyrene	0.00	202	0	N.D.	
64)	Butylbenzylphthalate	0.00	149	0	N.D.	
65)	Benzo(a)anthracene	33.05	228	2990	N.D.	
66)	Bis(2-ethylhexyl)phthalate	33.34	149	709	N.D.	
67)	Chrysene	33.05	228	2990	N.D.	
69)	Di-n-Octylphthalate	0.00	149	0	N.D.	
70)	Benzo(b)fluoranthene	0.00	252	0	N.D.	

(#) = qualifier out of range (m) = manual integration

Quantitation Report (QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV0901\25260.D Vial: 10
Acq On : 9 Nov 2001 9:13 pm Operator: 209 GALOS
Sample : gc/ms unknown Inst : GC/MS 209
Misc : Multiplr: 1.00
MS Integration Params: RTEINT.P
Quant Time: Nov 9 22:01 2001 Quant Results File: NP103001.RES

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Fri Nov 02 16:41:16 2001
Response via : Initial Calibration
DataAcq Meth : NP103001

	Compound	R.T.	QIon	Response	Conc Unit	Qvalue
71)	Benzo(k)fluoranthene	0.00	252	0	N.D.	
72)	Benzo(a)pyrene	37.16	252	3854	N.D.	
73)	Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.	
74)	Dibenz(a,h)anthracene	0.00	278	0	N.D.	
75)	Benzo(g,h,i)perylene	0.00	276	0	N.D.	

(#) = qualifier out of range (m) = manual integration

Quantitation Report

Data File : C:\HPCHEM\1\DATA\NOV0901\25260.D
Acq On : 9 Nov 2001 9:13 pm
Sample : gc/ms unknown
Misc :
MS Integration Params: RTEINT.P
Quant Time: Nov 9 22:01 2001

Vial: 10
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: NP103001.RES

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Tue Nov 27 12:20:14 2001
Response via : Initial Calibration

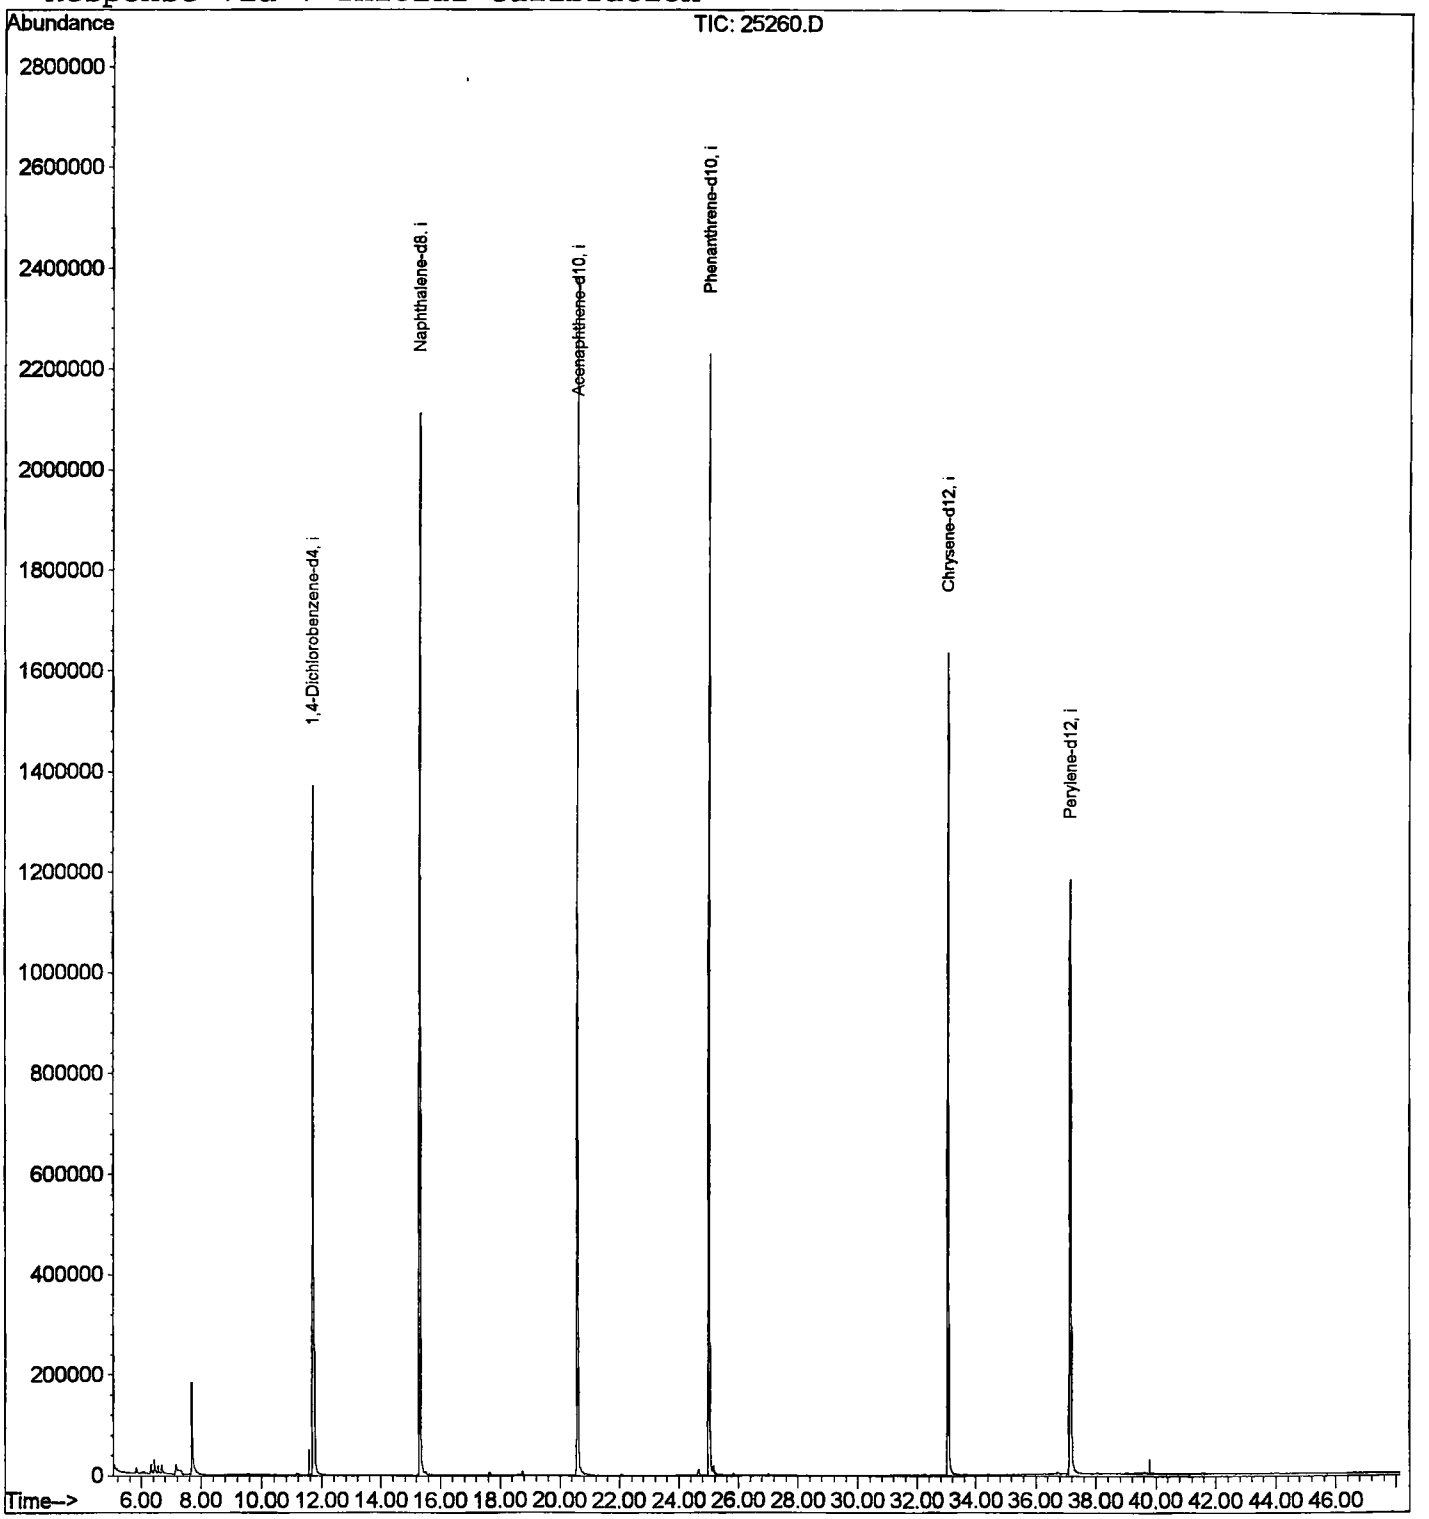

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\NOV0901\25260.D
Acq On : 9 Nov 2001 9:13 pm
Sample : gc/ms unknown
Misc :
MS Integration Params: LSCINT.P

Vial: 10
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Smoothing : OFF
Filtering: 5
Sampling : 1
Min Area: 1 % of largest Peak
Start Thrs: 0.2
Max Peaks: 100
Stop Thrs : 0
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	6.438	148	152	162	rVV	27673	68117	1.34%	0.265%
2	7.163	225	231	237	rBV2	18405	58778	1.16%	0.229%
3	7.686	285	288	307	rBV	182461	468409	9.21%	1.826%
4	11.707	721	726	748	rBV	1370215	3330754	65.48%	12.981%
5	15.315	1113	1119	1138	rBV	2112001	4520826	88.87%	17.619%
6	20.594	1687	1694	1711	rBV	2383042	5086833	100.00%	19.825%
7	25.019	2169	2176	2187	rBV2	2228042	4849299	95.33%	18.900%
8	25.156	2188	2191	2206	rVB2	17495	61382	1.21%	0.239%
9	33.051	3044	3051	3066	rBV2	1635597	3877954	76.24%	15.114%
10	37.155	3490	3498	3512	rBV2	1182480	3335868	65.58%	13.001%

Sum of corrected areas: 25658220

25260.D NP103001.M Tue Nov 27 12:27:45 2001

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\NOV0901\25260.D
Operator : 209 GALOS
Acquired : 9 Nov 2001 9:13 pm using AcqMethod NP103001
Instrument : GC/MS 209
Sample Name: gc/ms unknown
Misc Info :
Vial Number: 10
Quant File :NP103001.RES (RTE Integrator)

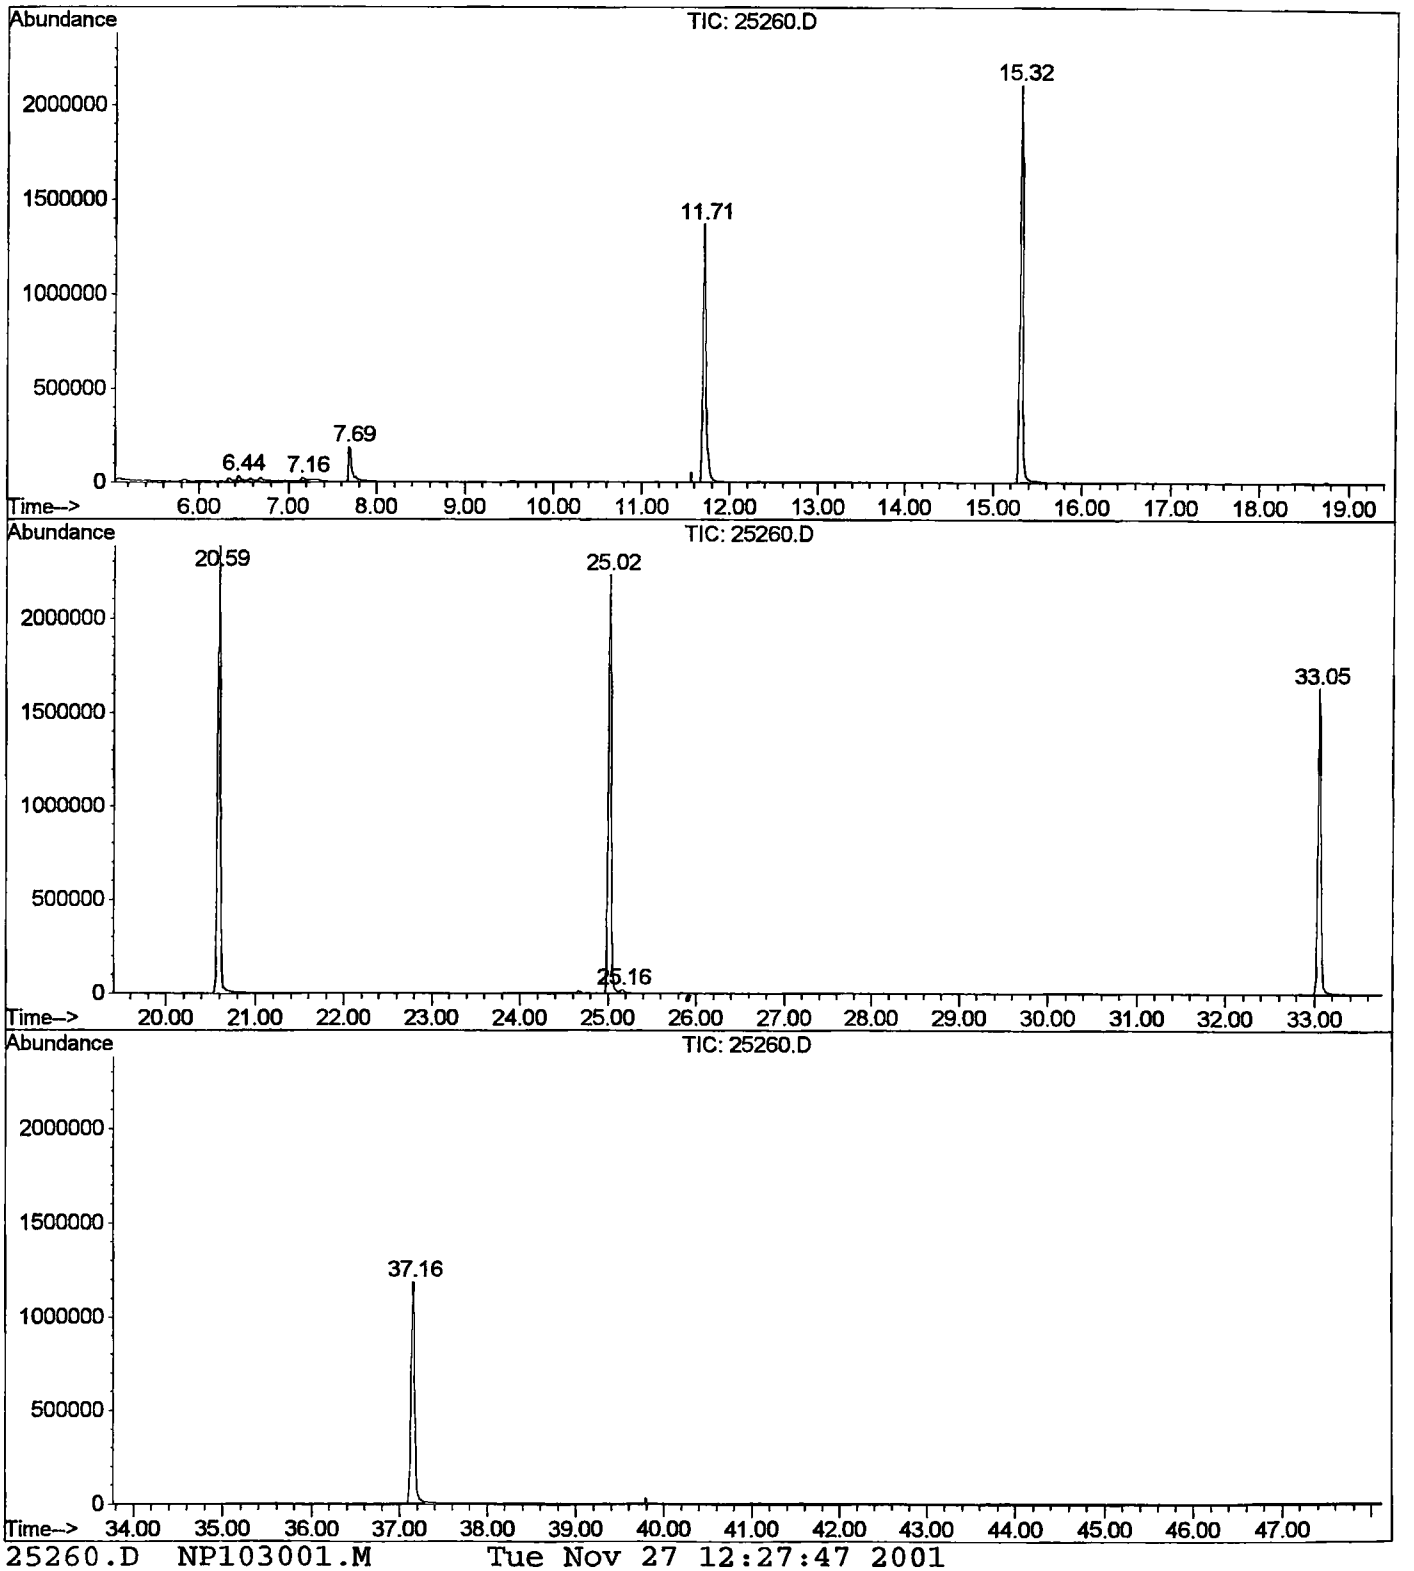

25260.D NP103001.M Tue Nov 27 12:27:47 2001

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\NOV0901\25260.D
Acq On : 9 Nov 2001 9:13 pm
Sample : gc/ms unknown
Misc :
MS Integration Params: LSCINT.P

Vial: 10
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

****

Peak Number 1 2-Hexanone Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.44	0.41 ug/l	68117	1,4-Dichlorobenzene-d4	11.71

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Hexanone	100	C6H12O	000591-78-6	91
2	2-Hexanone, 4-hydroxy-5-methyl-3-pr	172	C10H20O2	061141-74-0	64
3	2-Hexanone, 4-hydroxy-3-propyl-	158	C9H18O2	062338-17-4	64
4	Methyl Isobutyl Ketone	100	C6H12O	000108-10-1	58

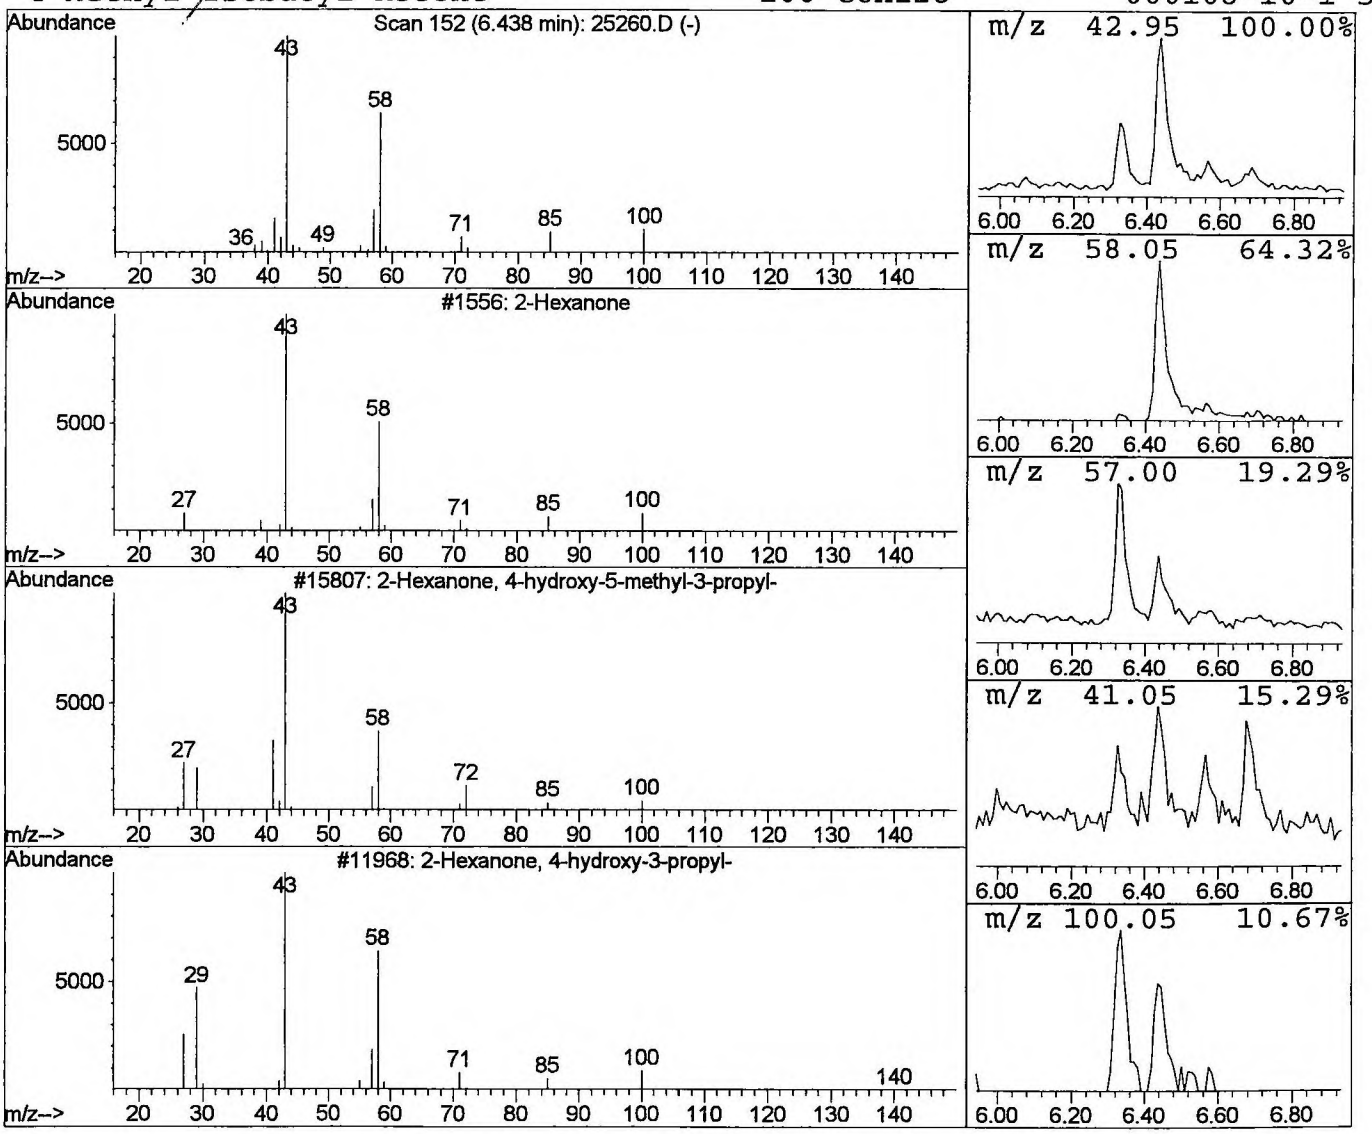

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\NOV0901\25260.D
Acq On : 9 Nov 2001 9:13 pm
Sample : gc/ms unknown
Misc :
MS Integration Params: LSCINT.P

Vial: 10
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

****

Peak Number 2 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.69	2.81 ug/l	468409	1,4-Dichlorobenzene-d4	11.71

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50
2	Acetic acid, 1,1-dimethylethyl este	116	C6H12O2	000540-88-5	33
3	Acetone	58	C3H6O	000067-64-1	10
4	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9

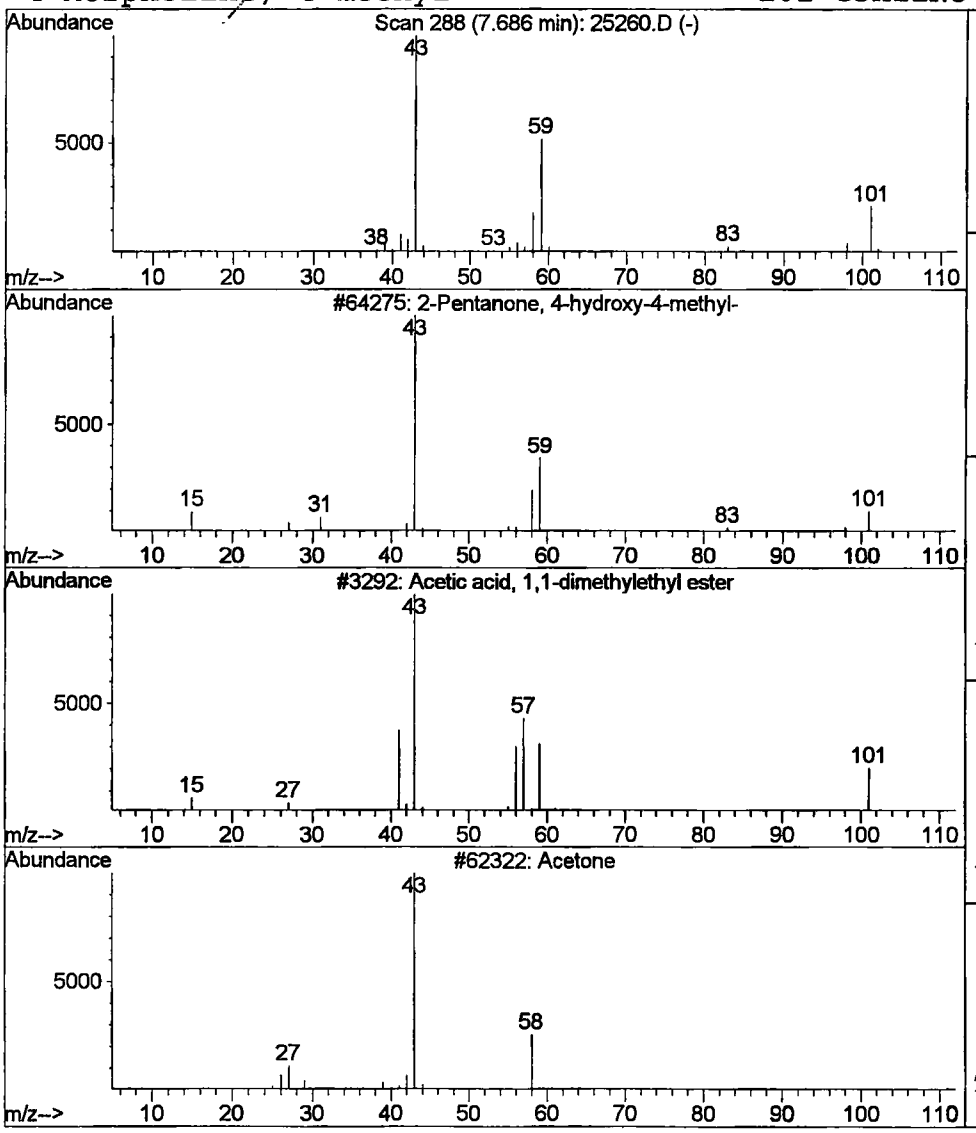

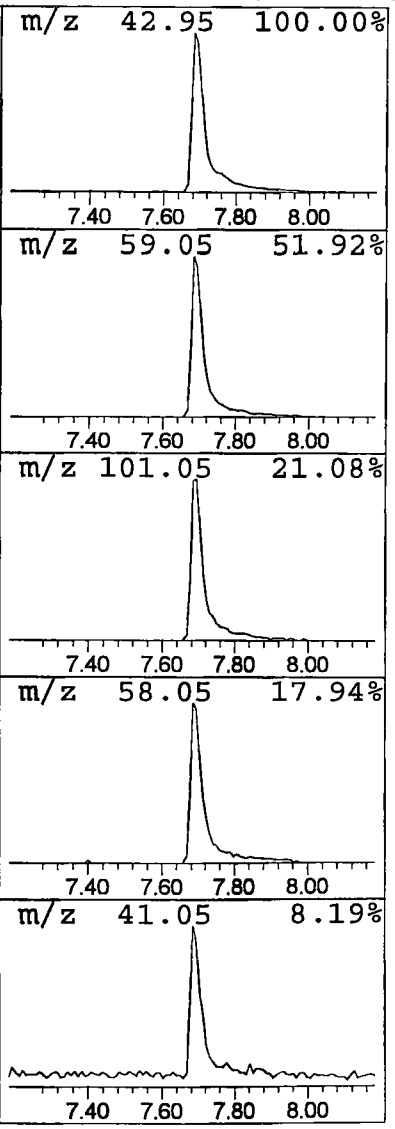

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 9 Nov 2001 9:13 pm
Data File: C:\HPCHEM\1\DATA\NOV0901\25260.D
Name: gc/ms unknown
Misc:
Method: C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Hexanone	6.44	0.4	ug/l	68117	ISTD01	11.71	3330750	20.0
2-Pentanone, 4-hydro	7.69	2.8	ug/l	468409	ISTD01	11.71	3330750	20.0

25260.D NP103001.M Tue Nov 27 12:27:54 2001