

Method 508
GCMS

Date Extracted 10/24/01

Page 47

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
	Lab blank	500µl	—	1µl		—	2µl		7			
	Reference POC phen											
	MDL POC											
	PRE 1016											
	25174									1		
	25175									2		
25175	spike post				1µl							WHID well #1
25175	spike post											WHID
25174	spike tox											well #2
25174	spike tox											
	25156 ✓									3		
	25259 ✓ 455									4		
	25045 ✓ 500µl									5		
	25264 ✓									6		
	25265 ✓									7		
	25375 ✓									8		
	25173 ✓									9		
	25174 ✓									10		
	25175 ✓									11		
	25176 ✓									12		
	25177 ✓									13		
	25178 ✓									14		
Remarks 25045 re-extracted Reviewed by, <u>15/12/02</u>												
drip rate must be between 5-15 ml/min for liq-liq extractors drip rate - Extraction type - <u>Sep funnel</u> Solv. lot# <u>V11599</u> Na2SO4 lot# <u>V32603</u>												
STANDARD	INT STD LOG#											
CALIBRATION												
REF/SPIKE	20622											
MDL/MDRF												
Q. CHECK												
INT. STD.												
SURROGATE	20646											
LPC												
ENDRIN/DDT												

Analyst mw/ml/AD
revision 4/12/01

Verified by _____

Reviewed by DN
Date 12/5/11

Sequence Name: C:\HPCHEM\1\SEQUENCE\NOV0901.S

Comment: INST 209; 30Mx0.25umX0.50

Operator: 209 GALOS

Data Path: C:\HPCHEM\1\data\nov0901\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run

☒ Full Method☐ Reprocessing Only

On A Barcode Mismatch

☒ Inject Anyway☐ Don't Inject

Line Type	Vial	DataFile	Method	Sample Name
-----------	------	----------	--------	-------------

1 Sample	1	DFTPP	NP103001	
2 Sample	2	LB	NP103001	10/23
3 Sample	3	25155	NP103001	gc/ms unknown
4 Sample	4	25263	NP103001	gc/ms unknown
5 Sample	5	25049	NP103001	gc/ms unknown
6 Sample	6	25050	NP103001	gc/ms unknown
7 Sample	7	25051	NP103001	gc/ms unknown
8 Sample	8	25259	NP103001	gc/ms unknown
9 Sample	9	25154	NP103001	gc/ms unknown
10 Sample	10	25260	NP103001	gc/ms unknown
11 Sample	11	25261	NP103001	gc/ms unknown
12 Sample	12	25262	NP103001	gc/ms unknown
13 Sample	13	25072	NP103001	gc/ms unknown
14 Sample	14	25073	NP103001	gc/ms unknown
15 Sample	15	25052	NP103001	gc/ms unknown
16 Sample	16	LBB	NP103001	lb blk 10/23
17 Sample	17	25174	NP103001	gc/ms unknown
18 Sample	18	25175	NP103001	gc/ms unknown
19 Sample	19	25045✓	NP103001	gc/ms unknown
20 Sample	20	25178	NP103001	gc/ms unknown

10/24

Sequence Name: C:\HPCHEM\1\SEQUENCE\NOV1401.S
Comment: INST 209; 30Mx0.25umX0.50
Operator: 209 GALOS
Data Path: C:\HPCHEM\1\data\nov0601\
Pre-Seq Cmd:
Post-Seq Cmd:

Method Sections To Run	On A Barcode Mismatch
(X) Full Method	(X) Inject Anyway
() Reprocessing Only	() Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	NP103001	
2	Sample	2	25156✓	NP103001	gc/ms unknown
3	Sample	3	25173	NP103001	gc/ms unknown
4	Sample	4	25176	NP103001	gc/ms unknown
5	Sample	5	25177	NP103001	gc/ms unknown
6	Sample	6	25264✓	NP103001	gc/ms unknown
7	Sample	7	25265✓	NP103001	gc/ms unknown
8	Sample	8	25259✓	NP103001	gc/ms unknown
9	Sample	9	25375✓	NP103001	gc/ms unknown
10	Sample	10	LB	NP103001	10/25
11	Sample	11	25376	NP103001	gc/ms unknown
12	Sample	12	25377	NP103001	gc/ms unknown

DFTPP

Data File : C:\HPCHEM\1\DATA\NOV0901\DFTPP.D

Acq On : 9 Nov 2001 11:27 am

Sample :

Misc :

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

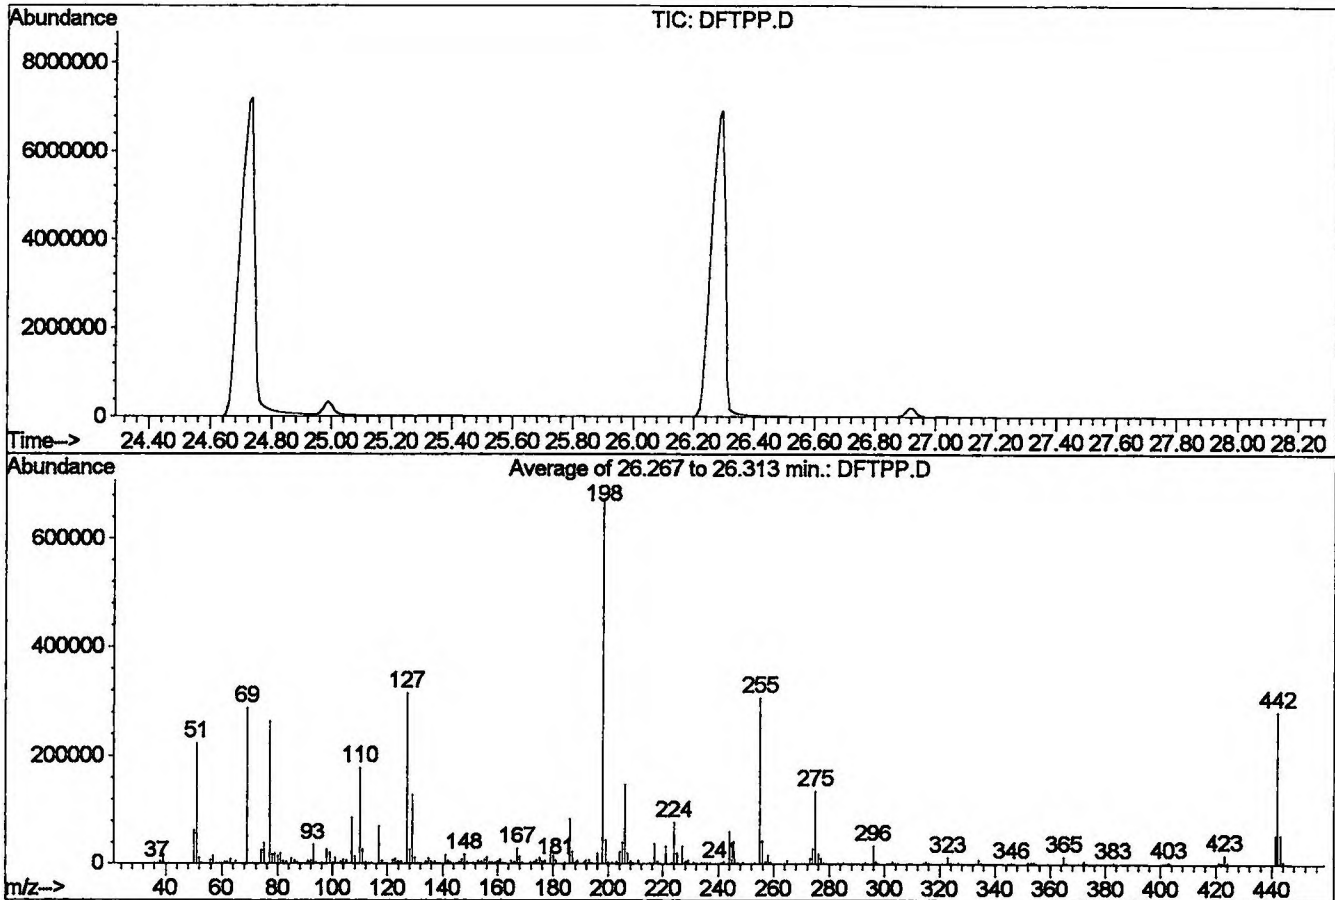

Spectrum Information: Average of 26.267 to 26.313 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	33.1	223091	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.7	287664	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	46.9	315453	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	673136	PASS
199	198	5	9	6.6	44325	PASS
275	198	10	30	20.2	136083	PASS
365	198	1	100	2.0	13271	PASS
441	443	0.01	100	97.4	52448	PASS
442	198	40	110	41.9	282336	PASS
443	442	17	23	19.1	53847	PASS

DFTPP.D NP103001.M

Wed Nov 28 12:52:25 2001

DFTPP

Data File : C:\HPCHEM\1\DATA\NOV1401\DFTPP.D

Acq On : 14 Nov 2001 4:38 pm

Sample :

Misc :

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

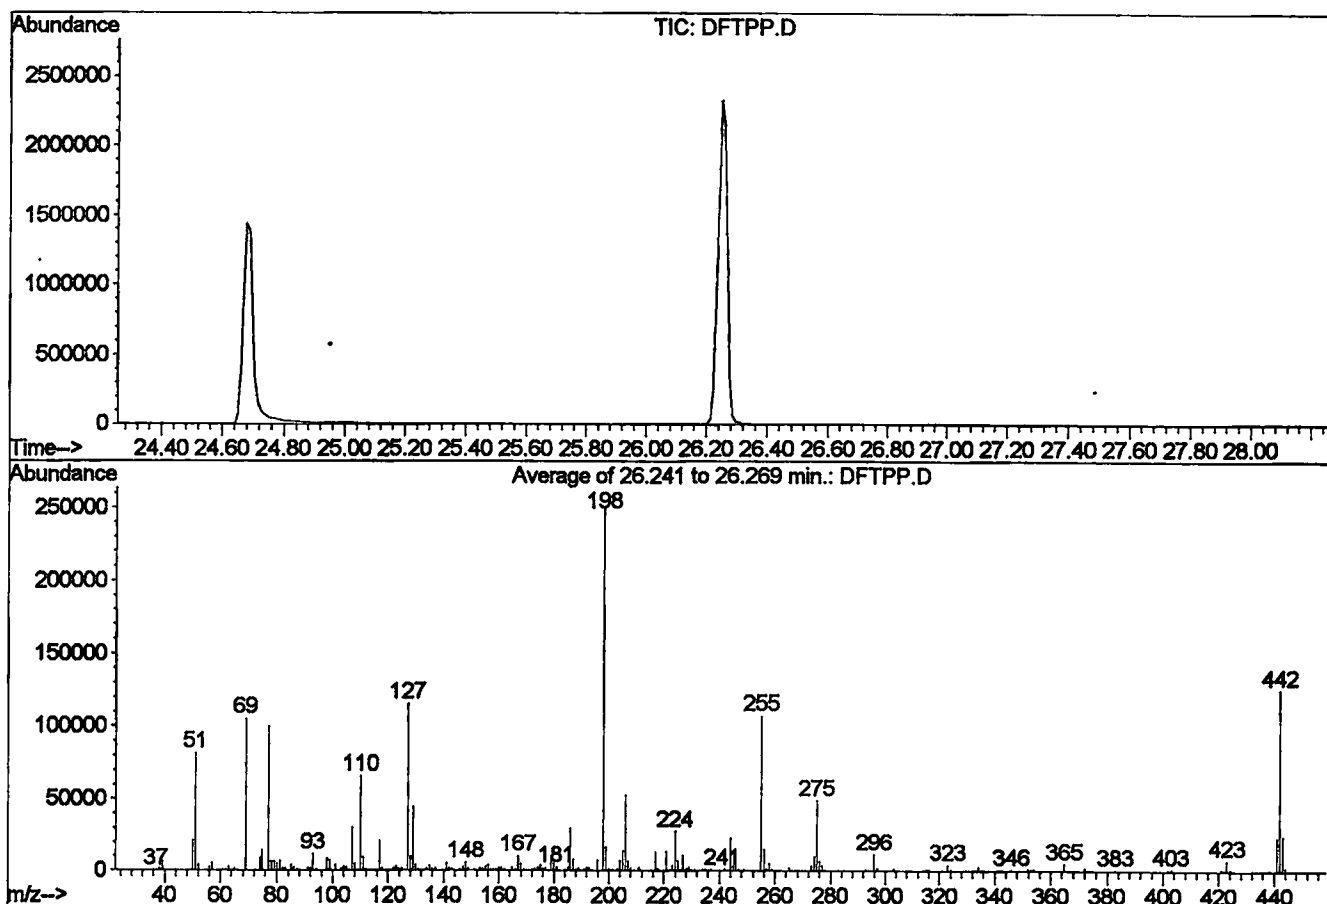

Spectrum Information: Average of 26.241 to 26.269 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	32.5	81646	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	41.9	105178	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	46.0	115456	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	251152	PASS
199	198	5	9	6.6	16498	PASS
275	198	10	30	19.6	49228	PASS
365	198	1	100	1.8	4643	PASS
441	443	0.01	100	95.0	22472	PASS
442	198	40	110	49.8	125086	PASS
443	442	17	23	18.9	23657	PASS

DFTPP.D NP103001.M

Wed Nov 28 12:35:30 2001