

Dr
12/7/11

Sequence Name: C:\HPCHEM\1\SEQUENCE\NOV1401.S

Comment: INST 209; 30Mx0.25umX0.50

Operator: 209 GALOS

Data Path: C:\HPCHEM\1\data\nov0601\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run	On A Barcode Mismatch
(X) Full Method	(X) Inject Anyway
() Reprocessing Only	() Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	NP103001	
2	Sample	2	25156	NP103001	gc/ms unknown
3	Sample	3	25173	NP103001	gc/ms unknown
4	Sample	4	25176	NP103001	gc/ms unknown
5	Sample	5	25177	NP103001	gc/ms unknown
6	Sample	6	25264	NP103001	gc/ms unknown
7	Sample	7	25265	NP103001	gc/ms unknown
8	Sample	8	25259	NP103001	gc/ms unknown
9	Sample	9	25375	NP103001	gc/ms unknown
10	Sample	10	LB ✓	NP103001	10/25
11	Sample	11	25376 ✓	NP103001	gc/ms unknown
12	Sample	12	25377 ✓	NP103001	gc/ms unknown

Sequence Name: C:\HPCHEM\1\SEQUENCE\NOV1501.S
Comment: INST 209; 30Mx0.25umX0.50
Operator: 209 GALOS
Data Path: C:\HPCHEM\1\data\nov0601\
Pre-Seq Cmd:
Post-Seq Cmd:

Method Sections To Run	On A Barcode Mismatch
(X) Full Method	(X) Inject Anyway
() Reprocessing Only	() Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	NP103001	
2	Sample	2	25459	NP103001	gc/ms unknown
3	Sample	3	25495	NP103001	gc/ms unknown
4	Sample	4	25460	NP103001	gc/ms unknown
5	Sample	5	25496	NP103001	gc/ms unknown

Sequence Name: C:\HPCHEM\1\SEQUENCE\NOV1601.S

Comment: INST 209; 30Mx0.25umX0.50

Operator: 209 GALOS

Data Path: C:\HPCHEM\1\data\nov1601\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run	On A Barcode Mismatch
(X) Full Method	(X) Inject Anyway
() Reprocessing Only	() Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	NP103001	
2	Sample	2	25603	NP103001	gc/ms unknown
3	Sample	3 25461 ✓		NP103001	gc/ms unknown
4	Sample	4 25497 ✓		NP103001	gc/ms unknown
5	Sample	5 25458 ✓		NP103001	gc/ms unknown
6	Sample	6 25463 ✓		NP103001	gc/ms unknown
7	Sample	7 25457 ✓		NP103001	gc/ms unknown
8	Sample	8 25462 ✓		NP103001	gc/ms unknown
9	Sample	9 LB		NP103001	lb 10/27
10	Sample	10 25599		NP103001	gc/ms unknown
11	Sample	11 25600		NP103001	gc/ms unknown
12	Sample	12 25601		NP103001	gc/ms unknown
13	Sample	13 25604		NP103001	gc/ms unknown
14	Sample	14 25602		NP103001	gc/ms unknown
15	Sample	15 25733		NP103001	gc/ms unknown
16	Sample	16 25665		NP103001	gc/ms unknown
17	Sample	17 25732		NP103001	gc/ms unknown
18	Sample	18 25735		NP103001	gc/ms unknown
19	Sample	19 25664		NP103001	gc/ms unknown
20	Sample	20 25734		NP103001	gc/ms unknown
21	Sample	21 25791		NP103001	gc/ms unknown
22	Sample	22 25605		NP103001	gc/ms unknown
23	Sample	23 25736		NP103001	gc/ms unknown
24	Sample	24 25738		NP103001	gc/ms unknown
25	Sample	25 24216FB		NP103001	gc/ms unknown field blk
26	Sample	26 24401FB		NP103001	gc/ms unknown field blk
27	Sample	27 25663		NP103001	gc/ms unknown
28	Sample	28 25737		NP103001	gc/ms unknown
29	Sample	29 LBB		NP103001	lb 10/29

DFTPP

Data File : C:\HPCHEM\1\DATA\NOV1401\DFTPP.D

Acq On : 14 Nov 2001 4:38 pm

Sample :

Misc :

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

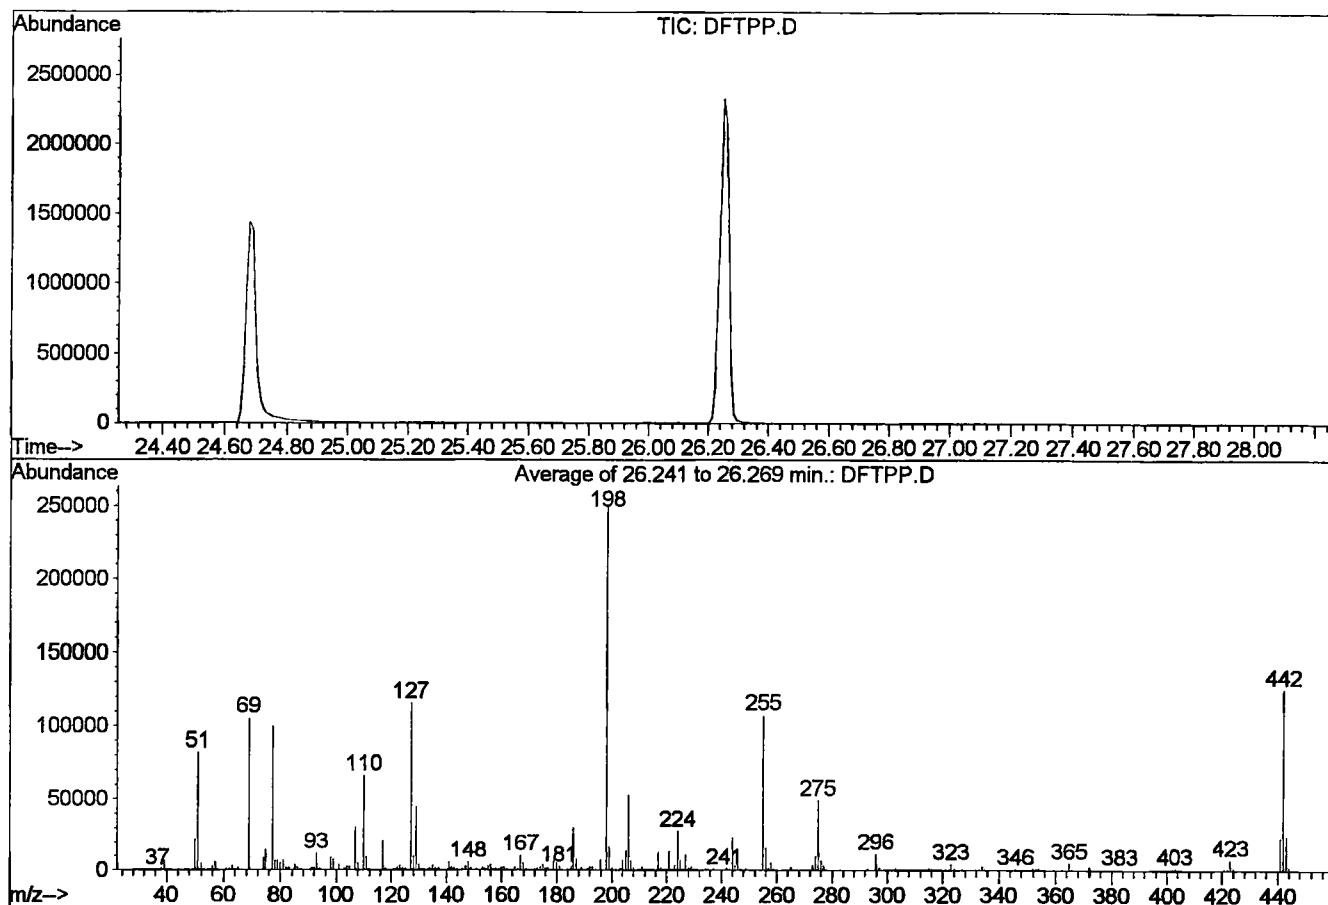

Spectrum Information: Average of 26.241 to 26.269 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	32.5	81646	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	41.9	105178	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	46.0	115456	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	251152	PASS
199	198	5	9	6.6	16498	PASS
275	198	10	30	19.6	49228	PASS
365	198	1	100	1.8	4643	PASS
441	443	0.01	100	95.0	22472	PASS
442	198	40	110	49.8	125086	PASS
443	442	17	23	18.9	23657	PASS

DFTPP.D NP103001.M

Fri Nov 16 14:55:24 2001

DFTPP

Data File : C:\HPCHEM\1\DATA\NOV1501\DFTPP.D

Acq On : 15 Nov 2001 4:18 pm

Sample :


Misc :

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Vial: 1
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

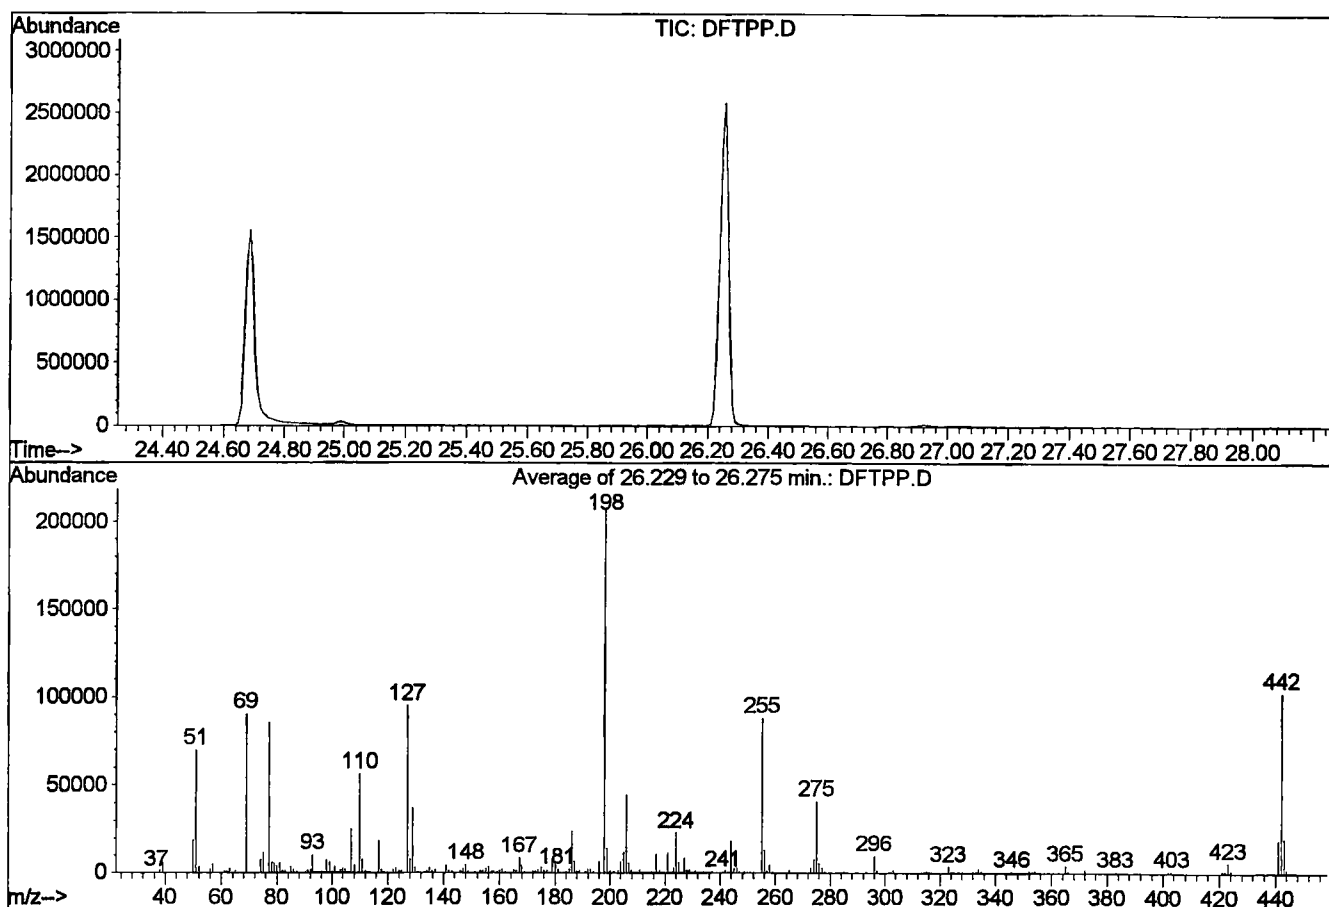

Spectrum Information: Average of 26.229 to 26.275 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	33.5	69757	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.5	90476	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	45.8	95299	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	207985	PASS
199	198	5	9	6.8	14059	PASS
275	198	10	30	19.6	40830	PASS
365	198	1	100	1.9	3859	PASS
441	443	0.01	100	94.0	18452	PASS
442	198	40	110	49.5	102872	PASS
443	442	17	23	19.1	19626	PASS

DFTPP.D NP103001.M

Fri Nov 16 14:55:49 2001