

Method 508 GUMBDate Extracted 10/27/01Page

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count
	LB	300ml		1ml			2ml		7	
	REF CH				1ml					
	MDL CH				1ml					
	PRL 1232				1ml					
	25599									6
	25600									7
	25601									8
	25602									9
	25603									10
	25604									11
Remarks										
Reviewed by: <u>SLB</u> 1/20/02										
drip rate must be between 5-15 ml/min for liq-liq extractors										
drip rate -										
Extraction type - <u>Sep Funnel</u> Solv. lot# <u>V29E66</u> NaCl lot# <u>V11899</u> Na2SO4 lot# <u>V32603</u>										
STANDARD	INT STD LOG#									
CALIBRATION										
REF/SPIKE	<u>Chloroform 1993</u>									
MDL/MDRF										
Q. CHECK										
INT. STD.										
SURROGATE	<u>2064L</u>									
LPC										
ENDRIN/DDT										

Analyst C.M.
revision 4/12/01Verified by Reviewed by DP
Date 12/7/11

Sequence Name: C:\HPCHEM\1\SEQUENCE\NOV1601.S

Comment: INST 209; 30Mx0.25umX0.50

Operator: 209 GALOS

Data Path: C:\HPCHEM\1\data\nov1601\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run

On A Barcode Mismatch

☒ Full Method☒ Inject Anyway☐ Reprocessing Only☐ Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	NP103001	
2	Sample	2	25603✓	NP103001	gc/ms unknown
3	Sample	3	25461	NP103001	gc/ms unknown
4	Sample	4	25497	NP103001	gc/ms unknown
5	Sample	5	25458	NP103001	gc/ms unknown
6	Sample	6	25463	NP103001	gc/ms unknown
7	Sample	7	25457	NP103001	gc/ms unknown
8	Sample	8	25462	NP103001	gc/ms unknown
9	Sample	9	LB	NP103001	lb 10/27
10	Sample	10	25599✓	NP103001	gc/ms unknown
11	Sample	11	25600✓	NP103001	gc/ms unknown
12	Sample	12	25601✓	NP103001	gc/ms unknown
13	Sample	13	25604✓	NP103001	gc/ms unknown
14	Sample	14	25602✓	NP103001	gc/ms unknown
15	Sample	15	25733	NP103001	gc/ms unknown
16	Sample	16	25665	NP103001	gc/ms unknown
17	Sample	17	25732	NP103001	gc/ms unknown
18	Sample	18	25735	NP103001	gc/ms unknown
19	Sample	19	25664	NP103001	gc/ms unknown
20	Sample	20	25734	NP103001	gc/ms unknown
21	Sample	21	25791	NP103001	gc/ms unknown
22	Sample	22	25605	NP103001	gc/ms unknown
23	Sample	23	25736	NP103001	gc/ms unknown
24	Sample	24	25738	NP103001	gc/ms unknown
25	Sample	25	24216FB	NP103001	gc/ms unknown field blk
26	Sample	26	24401FB	NP103001	gc/ms unknown field blk
27	Sample	27	25663	NP103001	gc/ms unknown
28	Sample	28	25737	NP103001	gc/ms unknown
29	Sample	29	LBB	NP103001	lb 10/29

DFTPP

Data File : C:\HPCHEM\1\DATA\NOV1601\DFTPP.D

Acq On : 16 Nov 2001 3:01 pm

Sample :

Misc :

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

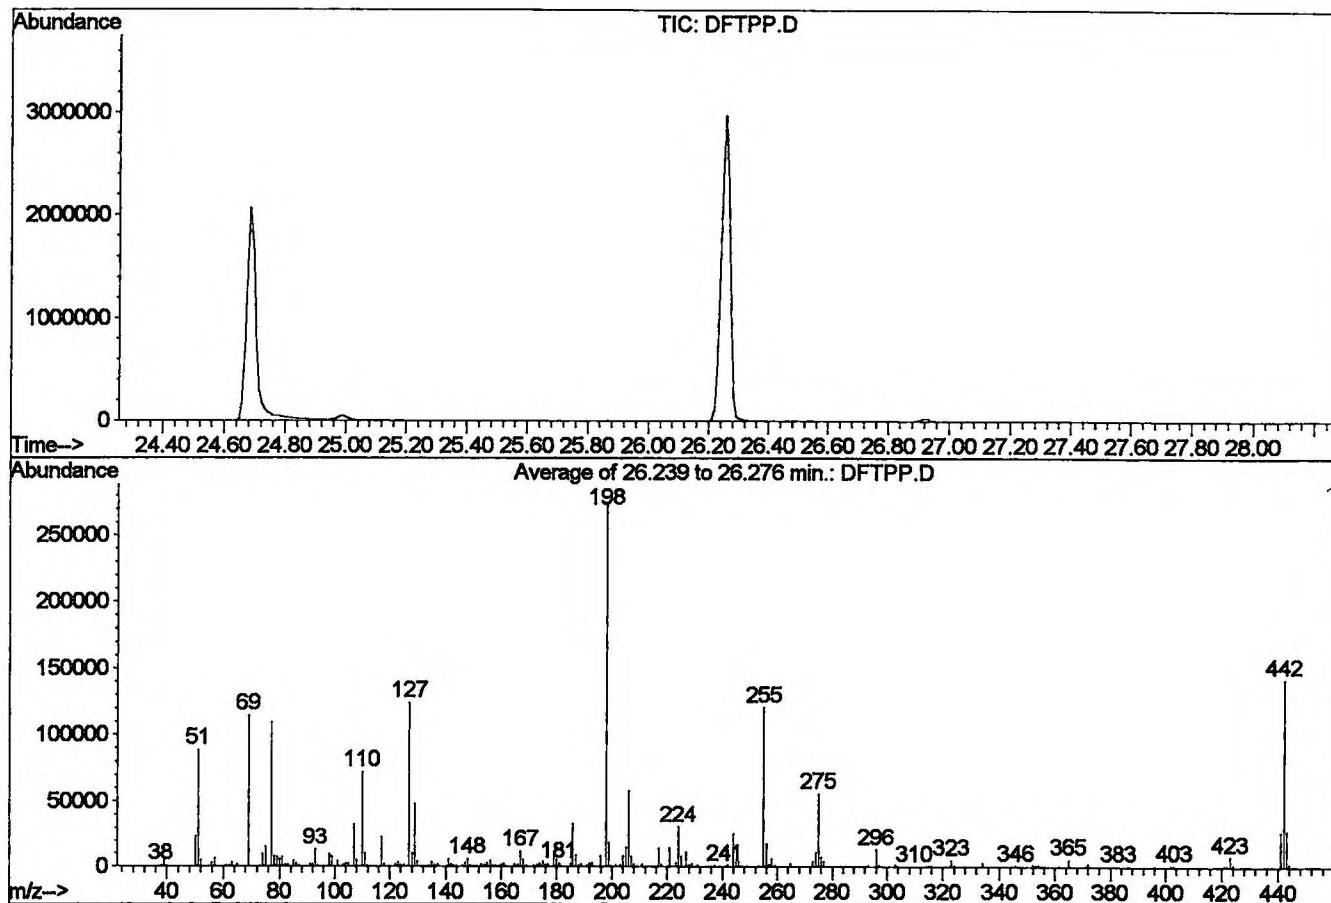

Spectrum Information: Average of 26.239 to 26.276 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	32.2	88587	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	41.7	114797	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	45.2	124325	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	274970	PASS
199	198	5	9	6.7	18386	PASS
275	198	10	30	20.4	56043	PASS
365	198	1	100	1.9	5306	PASS
441	443	0.01	100	95.0	25896	PASS
442	198	40	110	51.7	142195	PASS
443	442	17	23	19.2	27255	PASS

DFTPP.D NP103001.M

Mon Nov 19 11:38:45 2001