NYC 9/11 Public Portal Document

Method 508 GCMS  Date Extracted 10/29/01  Page _____

| Lab # | Description | Sample vol/wt | Drip rate ml/min | Surr add | Spk add | IS add | Final vol. | T.V. pos. | pH | Count | | |
|---|---|---|---|---|---|---|---|---|---|---|---|---|
| | LB | | | 1ml | | | 2ml | | | | | |
| | Ref tox | | | | 1ml | | | | | | | |
| | MDL tox | | | | 1ml | | | | | | | |
| | PQL 1242 | | | | 1ml | | | | | | | |
| | 256605 ✓ | | | | | | | | | 12 | | |
| | 256623 ✓ | | | | | | | | | 13 | | |
| | 256624 ✓ | | | | | | | | | 14 | | |
| | 256625 ✓ | | | | | | | | | 15 | | |
| | 25732 ✓ | | | | | | | | | 16 | | |
| | 25733 ✓ | | | | | | | | | 17 | | |
| | 25734 ✓ | | | | | | | | | 18 | | |
| | 25735 ✓ | | | | | | | | | 19 | | |
| | 25736 ✓ | | | | | | | | | 20 | | |
| | 25737 ✓ | | | | | | | | | 1 | | |
| | 25738 ✓ | | | | | | | | | 2 | | |
| | 25791 ✓ | | | | | | | | | 3 | | |
| 256605 | Spk tox | | | | 1ml | | | | | ~~4~~ | | |
| 256605 | Spk Dup tox | | | | 1ml | | | | | | | |
| 256605 | Spk pest | | | | 1ml | | | | | | | |
| 256623 | Spk Dup pest | | | ↓ | 1ml | | ↓ | | ↓ | | | |

**Remarks**

Reviewed by:

drip rate must be between 5-15 ml/min for liq-liq extractors  drip rate -

Extraction type - Sep Funnel  Solv.lot# V29E66  NaCl lot# V11599  Na2SO4 lot# V32603

| STANDARD | INT STD LOG# |
|---|---|
| CALIBRATION | |
| REF/SPIKE | 102 1992 pest - 2062 |
| MDL/MDRF | |
| Q. CHECK | |
| INT. STD. | |
| SURROGATE | 2064 |
| LPC | |
| ENDRIN/DDT | |

Analyst C.M./AD
revision 4/12/01

Verified by_____

Reviewed by_____
Date 12/7/11

NYC-WTC_000069815

Sequence Name: C:\HPCHEM\1\SEQUENCE\NOV1601.S
Comment: INST 209; 30Mx0.25umX0.50
Operator: 209 GALOS
Data Path: C:\HPCHEM\1\data\nov1601\
Pre-Seq Cmd:
Post-Seq Cmd:

Method Sections To Run
(X) Full Method
( ) Reprocessing Only

On A Barcode Mismatch
(X) Inject Anyway
( ) Don't Inject

| Line | Type | Vial | DataFile | Method | Sample Name |
|---|---|---|---|---|---|
| 1 | Sample | 1 | DFTPP | NP103001 | |
| 2 | Sample | 2 | 25603 | NP103001 | gc/ms unknown |
| 3 | Sample | 3 | 25461 | NP103001 | gc/ms unknown |
| 4 | Sample | 4 | 25497 | NP103001 | gc/ms unknown |
| 5 | Sample | 5 | 25458 | NP103001 | gc/ms unknown |
| 6 | Sample | 6 | 25463 | NP103001 | gc/ms unknown |
| 7 | Sample | 7 | 25457 | NP103001 | gc/ms unknown |
| 8 | Sample | 8 | 25462 | NP103001 | gc/ms unknown |
| 9 | Sample | 9 | LB | NP103001 | lb 10/27 |
| 10 | Sample | 10 | 25599 | NP103001 | gc/ms unknown |
| 11 | Sample | 11 | 25600 | NP103001 | gc/ms unknown |
| 12 | Sample | 12 | 25601 | NP103001 | gc/ms unknown |
| 13 | Sample | 13 | 25604 | NP103001 | gc/ms unknown |
| 14 | Sample | 14 | 25602 | NP103001 | gc/ms unknown |
| 15 | Sample | 15 | 25733 | NP103001 | gc/ms unknown |
| 16 | Sample | 16 | 25665 | NP103001 | gc/ms unknown |
| 17 | Sample | 17 | 25732 | NP103001 | gc/ms unknown |
| 18 | Sample | 18 | 25735 | NP103001 | gc/ms unknown |
| 19 | Sample | 19 | 25664 | NP103001 | gc/ms unknown |
| 20 | Sample | 20 | 25734 | NP103001 | gc/ms unknown |
| 21 | Sample | 21 | 25791 | NP103001 | gc/ms unknown |
| 22 | Sample | 22 | 25605 | NP103001 | gc/ms unknown |
| 23 | Sample | 23 | 25736 | NP103001 | gc/ms unknown |
| 24 | Sample | 24 | 25738 | NP103001 | gc/ms unknown |
| 25 | Sample | 25 | 24216FB | NP103001 | gc/ms unknown field blk |
| 26 | Sample | 26 | 24401FB | NP103001 | gc/ms unknown field blk |
| 27 | Sample | 27 | 25663 | NP103001 | gc/ms unknown |
| 28 | Sample | 28 | 25737 | NP103001 | gc/ms unknown |
| 29 | Sample | 29 | LBB | NP103001 | lb 10/29 |

Last Modified: Mon Nov 19 08:54:40 2001 Page: 1

NYC 9/11 Public Portal Document

# DFTPP

Data File : C:\HPCHEM\1\DATA\NOV1601\DFTPP.D
Acq On : 16 Nov 2001 3:01 pm
Sample :
Misc :
MS Integration Params: RTEINT.P
Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
Title : 209 625/TCLP calibration table

Vial: 1
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

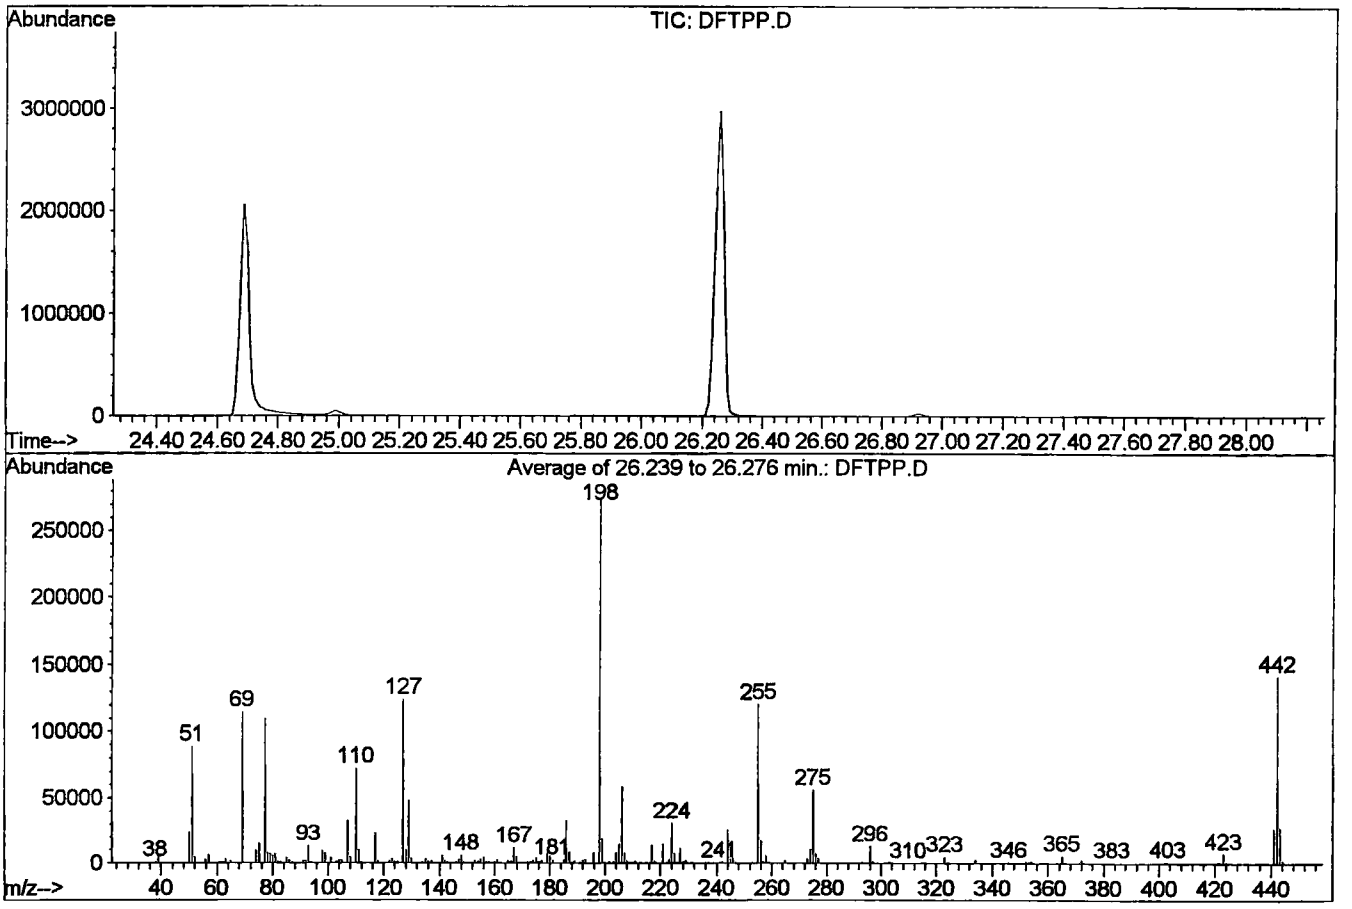


Spectrum Information: Average of 26.239 to 26.276 min.

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|---|---|---|---|---|---|---|
| 51 | 198 | 30 | 60 | 32.2 | 88587 | PASS |
| 68 | 69 | 0.00 | 2 | 0.0 | 0 | PASS |
| 69 | 198 | 0.00 | 100 | 41.7 | 114797 | PASS |
| 70 | 69 | 0.00 | 2 | 0.0 | 0 | PASS |
| 127 | 198 | 40 | 60 | 45.2 | 124325 | PASS |
| 197 | 198 | 0.00 | 1 | 0.0 | 0 | PASS |
| 198 | 198 | 100 | 100 | 100.0 | 274970 | PASS |
| 199 | 198 | 5 | 9 | 6.7 | 18386 | PASS |
| 275 | 198 | 10 | 30 | 20.4 | 56043 | PASS |
| 365 | 198 | 1 | 100 | 1.9 | 5306 | PASS |
| 441 | 443 | 0.01 | 100 | 95.0 | 25896 | PASS |
| 442 | 198 | 40 | 110 | 51.7 | 142195 | PASS |
| 443 | 442 | 17 | 23 | 19.2 | 27255 | PASS |

DFTPP.D NP103001.M Mon Nov 26 12:17:44 2001

NYC-WTC_000069817