

User: Galos, Marie
 Westchester Dept. of Labs & Research
 Date: 11/29/2001 Time: 14:51:55

Sample: AD25736
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 11/29/01 14:50 Ended: 11/29/01 14:50 Analyst: MG
 Page: 1

	Component Name	Viol	Result
1	Other unknown compounds		see comment

Comments for Sample AD25736 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Galos, Marie

Date: 11-29-2001 Time: 14:51:39

A scan of the extract prepared for the 508 analysis, from 35-550 amu using a mass spectrometer, does not reveal the presence of non-target compounds.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV1601\25736.D
 Acq On : 17 Nov 2001 12:30 pm
 Sample : gc/ms unknown
 Misc :
 MS Integration Params: RTEINT.P
 Quant Time: Nov 17 13:18 2001

Vial: 23
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: NP103001.RES

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Fri Nov 02 16:41:16 2001
 Response via : Initial Calibration
 DataAcq Meth : NP103001

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	11.71	152	618543	20.00	ug/l	-0.02
19) Naphthalene-d8	15.32	136	2326527	20.00	ug/l	-0.02
31) Acenaphthene-d10	20.59	164	1158692	20.00	ug/l	-0.02
49) Phenanthrene-d10	25.02	188	1706924	20.00	ug/l	-0.02
59) Chrysene-d12	33.05	240	1295050	20.00	ug/l	-0.02
68) Perylene-d12	37.16	264	965238	20.00	ug/l	0.00

System Monitoring Compounds

4) 2-Fluorophenol	0.00	112	0	0.00	ug/l	
Spiked Amount 75.000			Recovery	=	0.00%	
5) Phenol-d5	0.00	99	0	0.00	ug/l	
Spiked Amount 75.000			Recovery	=	0.00%	
6) 2-Chlorophenol-d4	0.00	132	0	0.00	ug/l	
Spiked Amount 75.000			Recovery	=	0.00%	
7) 1,2-Dichlorobenzene-d4	12.26	152	483	0.02	ug/l	0.01
Spiked Amount 50.000			Recovery	=	0.04%	
20) Nitrobenzene-d5	0.00	82	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
32) 2-Fluorobiphenyl	18.75	172	1646	0.02	ug/l	0.13
Spiked Amount 50.000			Recovery	=	0.04%	
33) 2,4,6-Tribromophenol	0.00	330	0	0.00	ug/l	
Spiked Amount 75.000			Recovery	=	0.00%	
62) Terphenyl-d14	0.00	244	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	

Target Compounds

					Qvalue
2) Pyridine	0.00	79	0	N.D.	
3) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
8) Phenol	0.00	94	0	N.D.	
9) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
10) 2-Chlorophenol	0.00	128	0	N.D.	
11) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
12) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
13) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
14) 2-Methylphenol	0.00	108	0	N.D.	
15) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
16) 3&4-Methylphenol	0.00	108	0	N.D.	
17) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
18) Hexachloroethane	0.00	117	0	N.D.	
21) Nitrobenzene	0.00	77	0	N.D.	
22) Isophorone	0.00	82	0	N.D.	

(#) = qualifier out of range (m) = manual integration
 25736.D NP103001.M Thu Nov 29 09:06:39 2001

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV1601\25736.D

Acq On : 17 Nov 2001 12:30 pm

Sample : gc/ms unknown

Misc :

MS Integration Params: RTEINT.P

Quant Time: Nov 17 13:18 2001

Vial: 23

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

Quant Results File: NP103001.RES

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Nov 02 16:41:16 2001

Response via : Initial Calibration

DataAcq Meth : NP103001

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
23) 2-Nitrophenol	0.00	139	0	N.D.		
24) 2,4-Dimethylphenol	0.00	107	0	N.D.		
25) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.		
26) 2,4-Dichlorophenol	0.00	162	0	N.D.		
27) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.		
28) Naphthalene	0.00	128	0	N.D.		
29) Hexachlorobutadiene	0.00	225	0	N.D.		
30) 4-Chloro-3-methylphenol	0.00	107	0	N.D.		
34) Hexachlorocyclopentadiene	0.00	237	0	N.D.		
35) 2,4,6-Trichlorophenol	0.00	196	0	N.D.		
36) 2,4,5-Trichlorophenol	0.00	196	0	N.D.		
37) 2-Chloronaphthalene	0.00	162	0	N.D.		
38) Dimethylphthalate	0.00	163	0	N.D.		
39) 2,6-Dinitrotoluene	0.00	165	0	N.D.		
40) Acenaphthylene	0.00	152	0	N.D.		
41) Acenaphthene	0.00	153	0	N.D.		
42) 2,4-Dinitrophenol	0.00	184	0	N.D.		
43) 4-Nitrophenol	0.00	65	0	N.D.		
44) 2,4-Dinitrotoluene	0.00	165	0	N.D.		
45) Diethylphthalate	0.00	149	0	N.D.		
46) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.		
47) Fluorene	0.00	166	0	N.D.		
48) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.		
50) 4,6-Dinitro-2-methylphenol	0.00	198	0	N.D.		
51) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
52) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
53) Hexachlorobenzene	0.00	284	0	N.D.		
54) Pentachlorophenol	0.00	266	0	N.D.		
55) Phenanthrene	25.08	178	275	N.D.		
56) Anthracene	25.08	178	275	N.D.		
57) Di-n-butylphthalate	27.03	149	2746	N.D.		
58) Fluoranthene	0.00	202	0	N.D.		
60) 3,3'-Dichlorobenzidine	0.00	252	0	N.D.		
61) Benzidine	0.00	184	0	N.D.		
63) Pyrene	0.00	202	0	N.D.		
64) Butylbenzylphthalate	0.00	149	0	N.D.		
65) Benzo(a)anthracene	33.05	228	3098	N.D.		
66) Bis(2-ethylhexyl)phthalate	33.33	149	1127	N.D.		
67) Chrysene	33.05	228	3098	N.D.		
69) Di-n-Octylphthalate	0.00	149	0	N.D.		
70) Benzo(b)fluoranthene	0.00	252	0	N.D.		

(#)=qualifier out of range (m)=manual integration

25736.D NP103001.M Thu Nov 29 09:06:44 2001

Page 2

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV1601\25736.D

Acq On : 17 Nov 2001 12:30 pm

Sample : gc/ms unknown

Misc :

MS Integration Params: RTEINT.P

Quant Time: Nov 17 13:18 2001

Vial: 23

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

Quant Results File: NP103001.RES

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Nov 02 16:41:16 2001

Response via : Initial Calibration

DataAcq Meth : NP103001

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
71) Benzo(k)fluoranthene	0.00	252	0	N.D.		
72) Benzo(a)pyrene	37.17	252	3641	N.D.		
73) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
74) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
75) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration
25736.D NP103001.M Thu Nov 29 09:06:45 2001

Page 3


Quantitation Report

Data File : C:\HPCHEM\1\DATA\NOV1601\25736.D
Acq On : 17 Nov 2001 12:30 pm
Sample : gc/ms unknown
Misc :
MS Integration Params: RTEINT.P
Quant Time: Nov 17 13:18 2001

Vial: 23
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: NP103001.RES

Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Fri Nov 02 16:41:16 2001
Response via : Initial Calibration

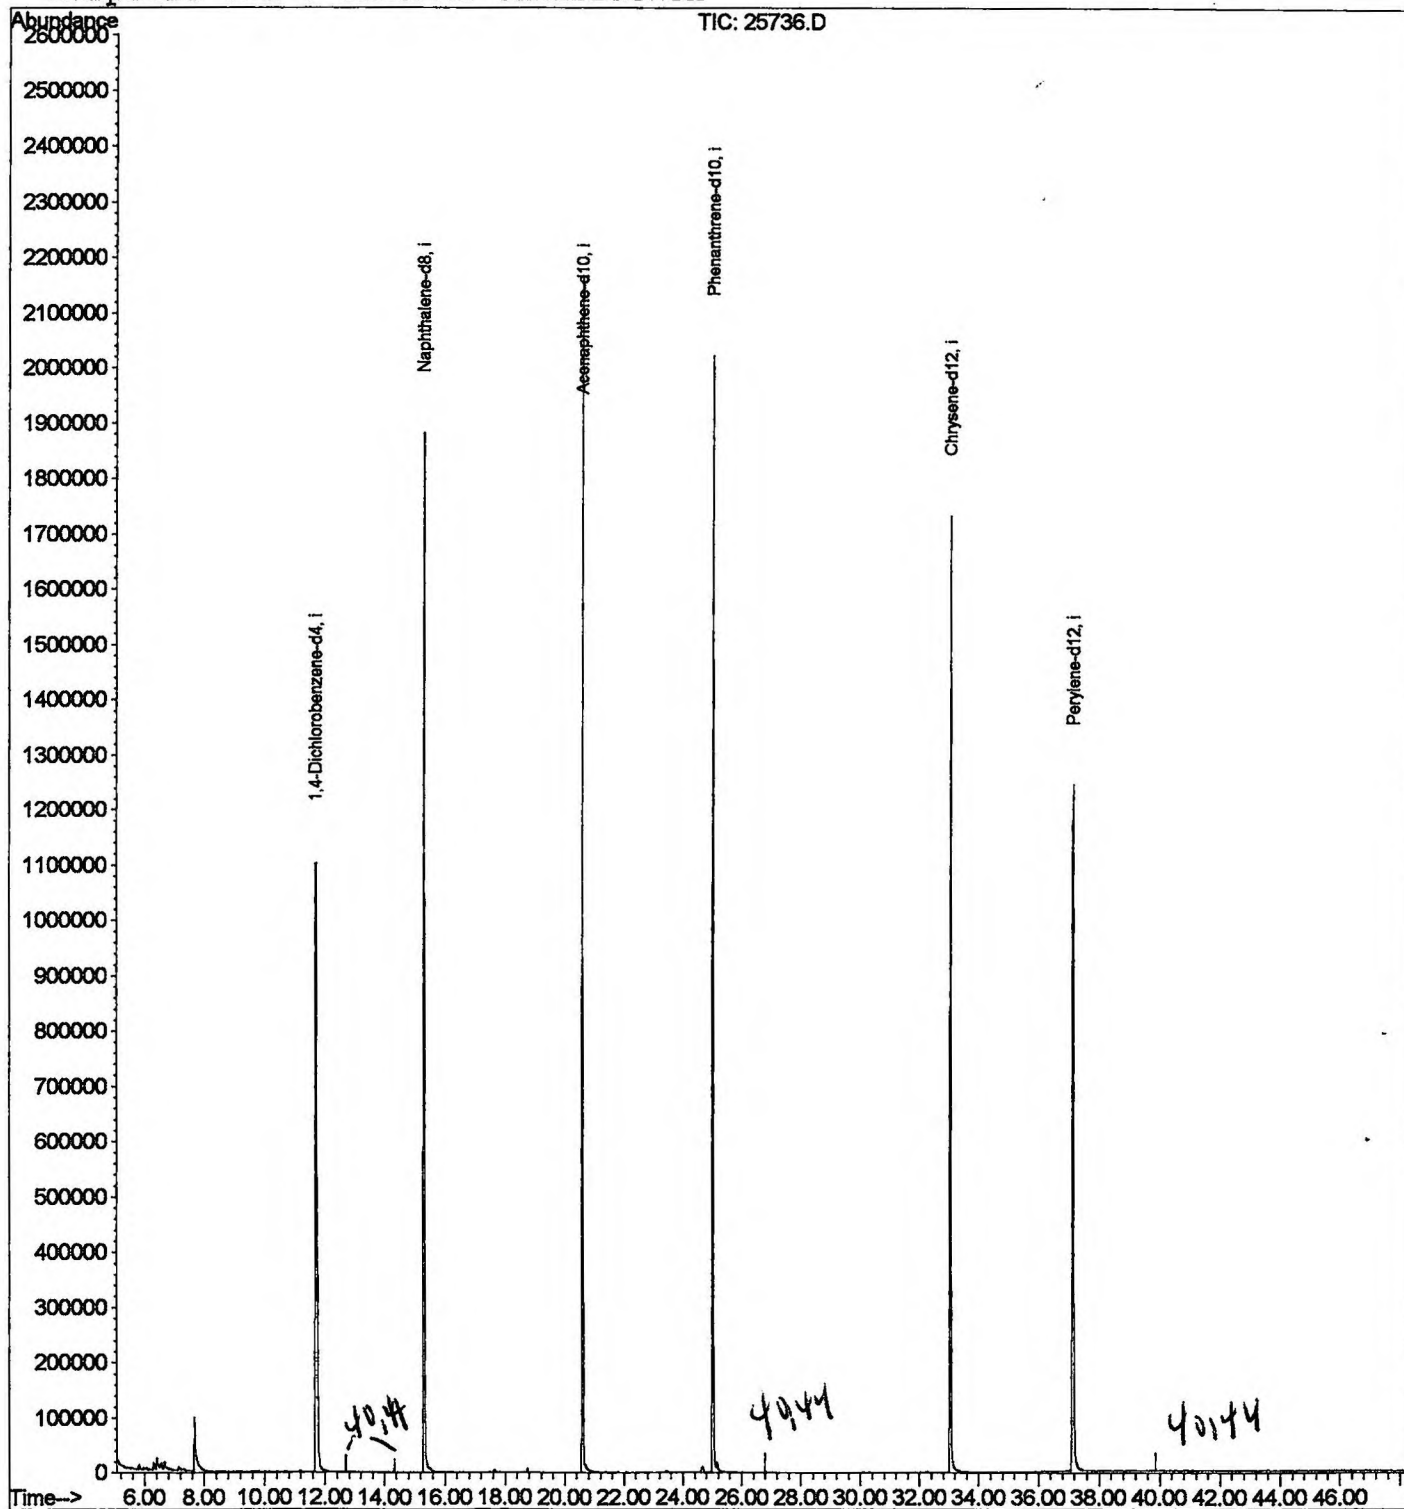

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\NOV1601\25736.D
 Acq On : 17 Nov 2001 12:30 pm
 Sample : gc/ms unknown
 Misc :
 MS Integration Params: LSCINT.P

Vial: 23
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC




peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	6.411	146	149	158	rVV	21247	68536	1.47%	0.277%
2	7.678	283	287	314	rBV	97573	389971	8.38%	1.577%
3	11.708	721	726	749	rBV	1103508	3209401	68.94%	12.975%
4	15.316	1114	1119	1138	rBV	1880855	4226874	90.80%	17.089%
5	20.595	1688	1694	1715	rBV	2167626	4655326	100.00%	18.821%
6	25.020	2169	2176	2187	rBV2	2021981	4438369	95.34%	17.944%
7	25.158	2188	2191	2204	rVB	17013	53689	1.15%	0.217%
8	33.053	3044	3051	3069	rBV2	1731992	4067432	87.37%	16.444%
9	37.156	3489	3498	3516	rBV2	1241129	3624750	77.86%	14.655%

Sum of corrected areas: 24734348

25736.D NP103001.M Thu Nov 29 09:21:18 2001

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\NOV1601\25736.D
 Operator : 209 GALOS
 Acquired : 17 Nov 2001 12:30 pm using AcqMethod NP103001
 Instrument : GC/MS 209
 Sample Name: gc/ms unknown
 Misc Info :
 Vial Number: 23
 Quant File :NP103001.RES (RTE Integrator)

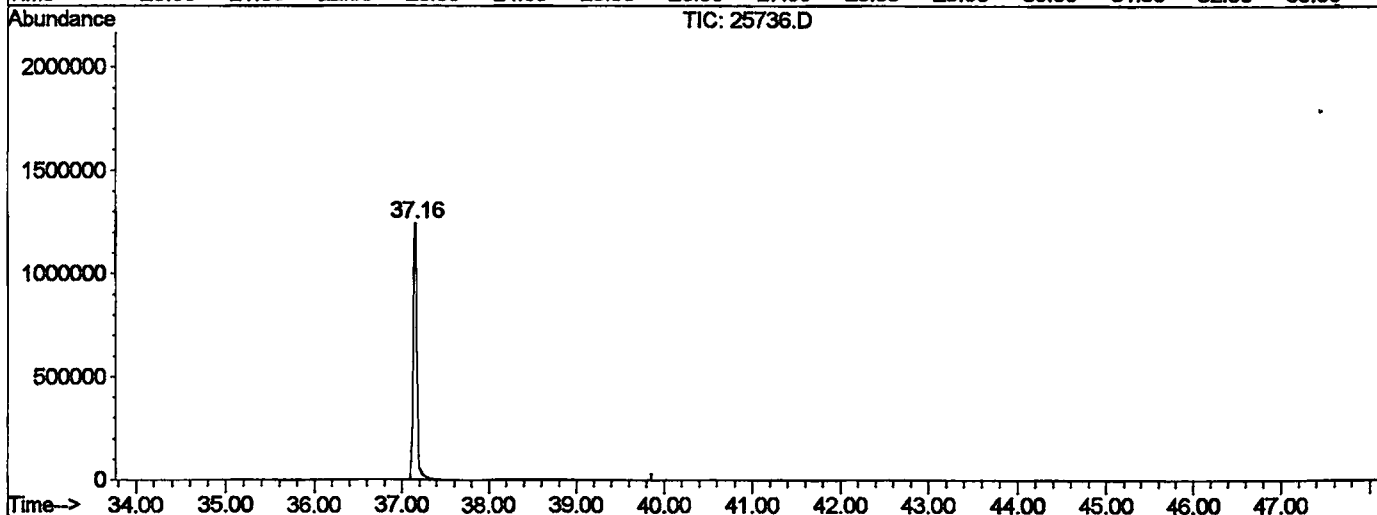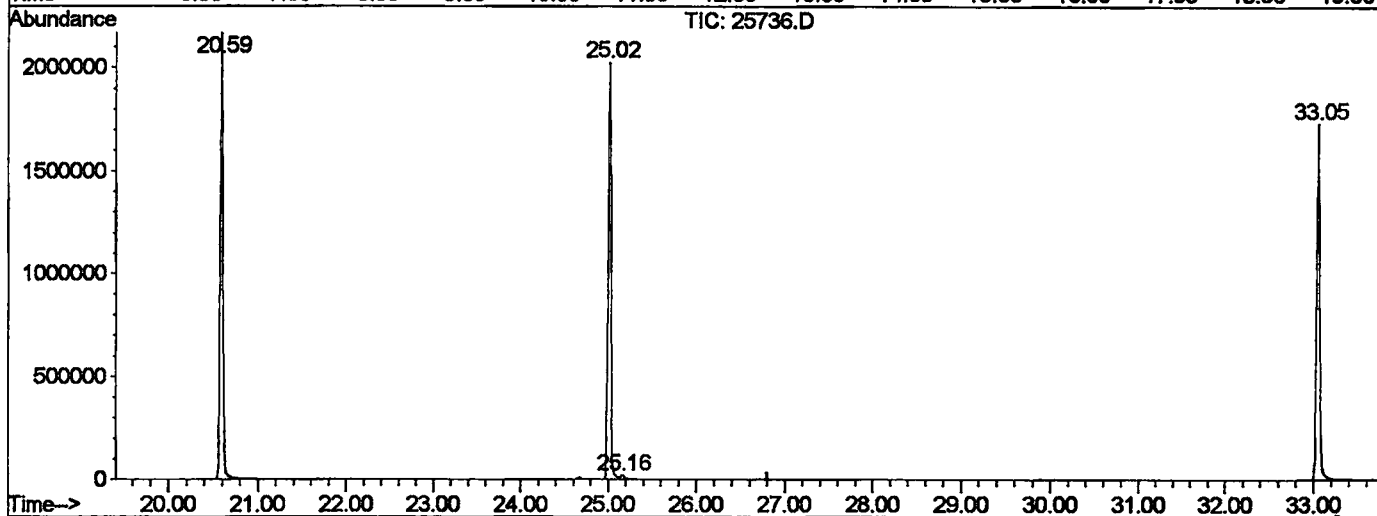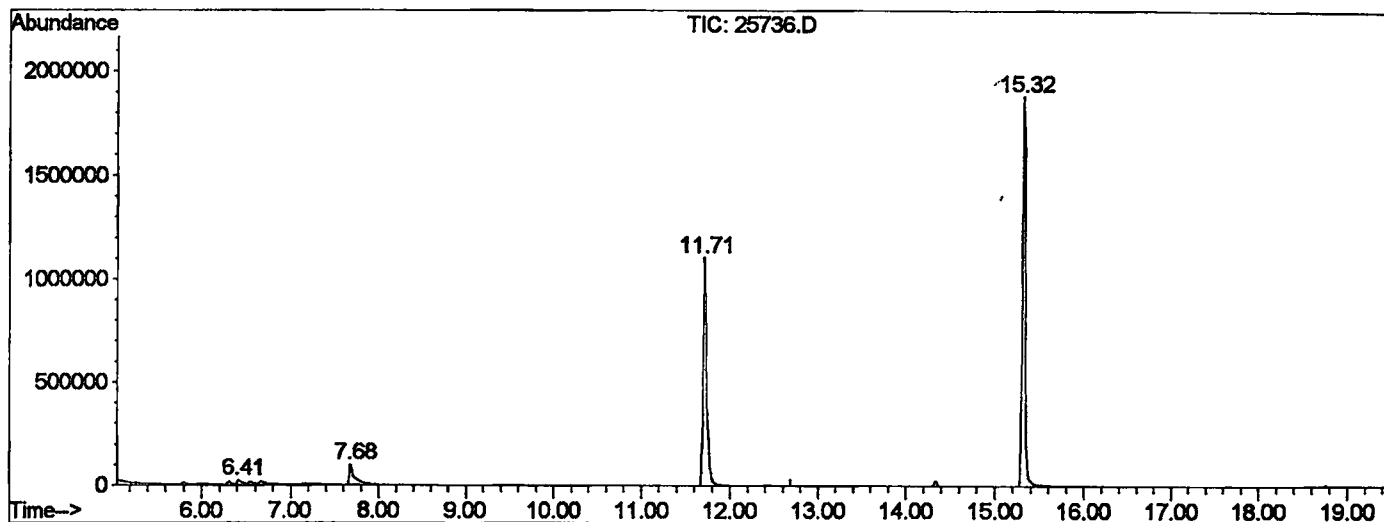

25736.D NP103001.M Thu Nov 29 09:21:21 2001

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\NOV1601\25736.D
 Acq On : 17 Nov 2001 12:30 pm
 Sample : gc/ms unknown
 Misc :
 MS Integration Params: LSCINT.P


Vial: 23
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 2-Hexanone Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.41	0.43 ug/l	68536	1,4-Dichlorobenzene-d4	11.71

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Hexanone	100	C6H12O	000591-78-6	87
2		2-Hexanone, 4-hydroxy-3-propyl-	158	C9H18O2	062338-17-4	64
3		Methyl Isobutyl Ketone	100	C6H12O	000108-10-1	52
4		2-Hexanone, 4-methyl-	114	C7H14O	000105-42-0	50

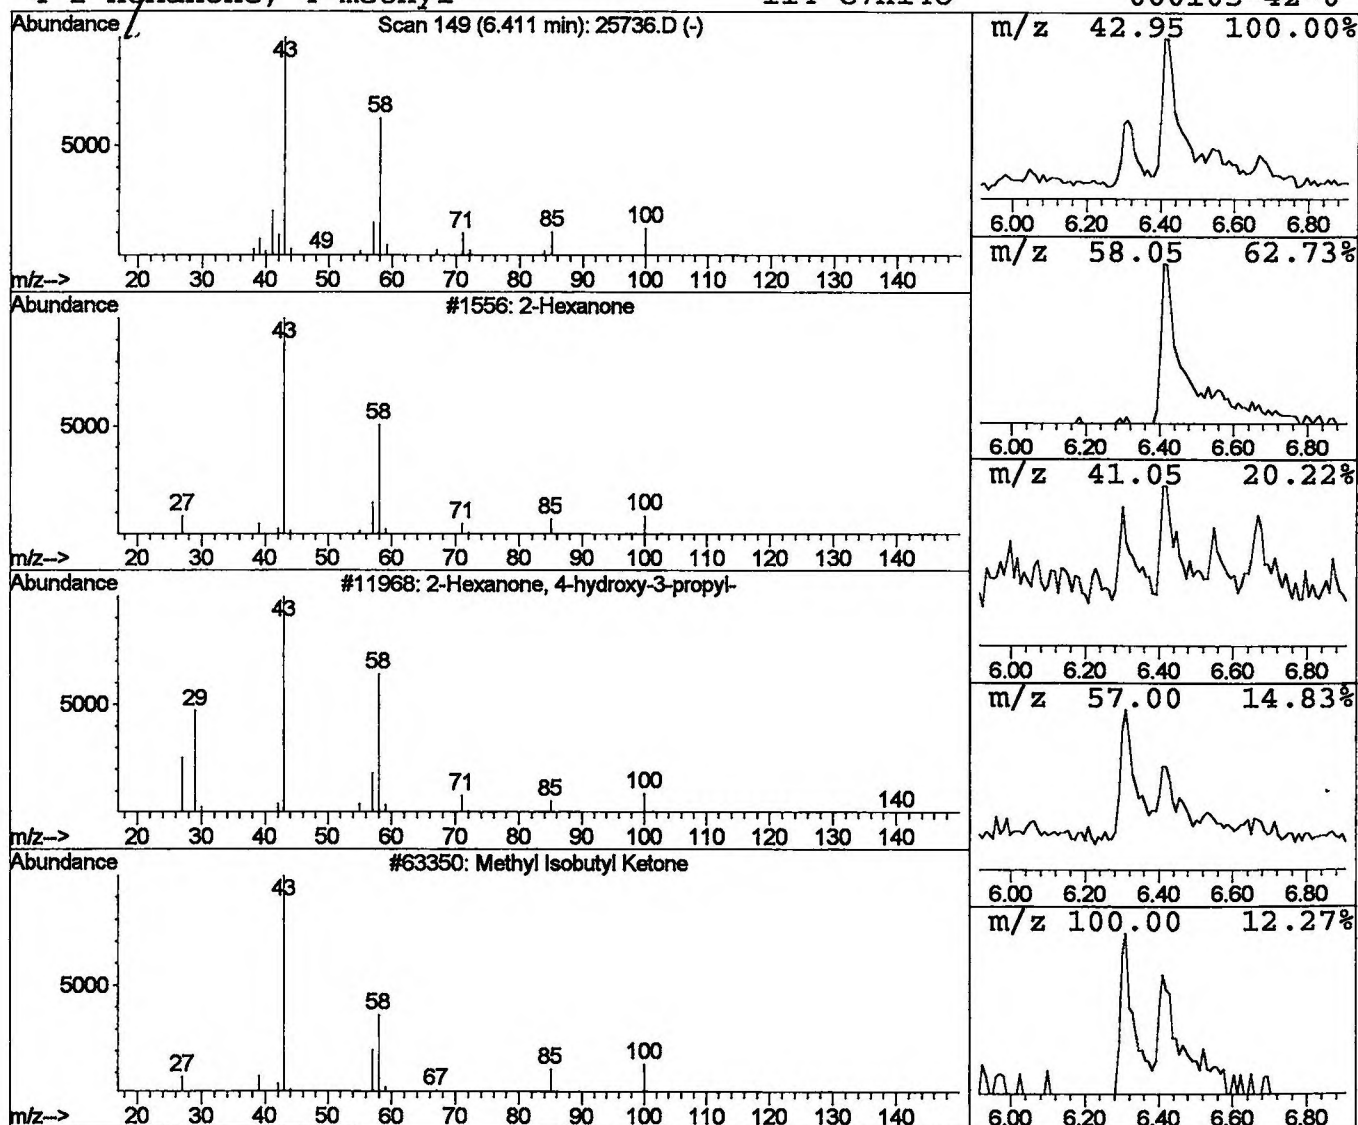

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\NOV1601\25736.D
Acq On : 17 Nov 2001 12:30 pm
Sample : gc/ms unknown
Misc :
MS Integration Params: LSCINT.P


Vial: 23
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 2 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.68	2.43 ug/l	389971	1,4-Dichlorobenzene-d4	11.71

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	72
2		Acetone	58	C3H6O	000067-64-1	12
3		Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9
4		5-Hexen-2-one	98	C6H10O	000109-49-9	9

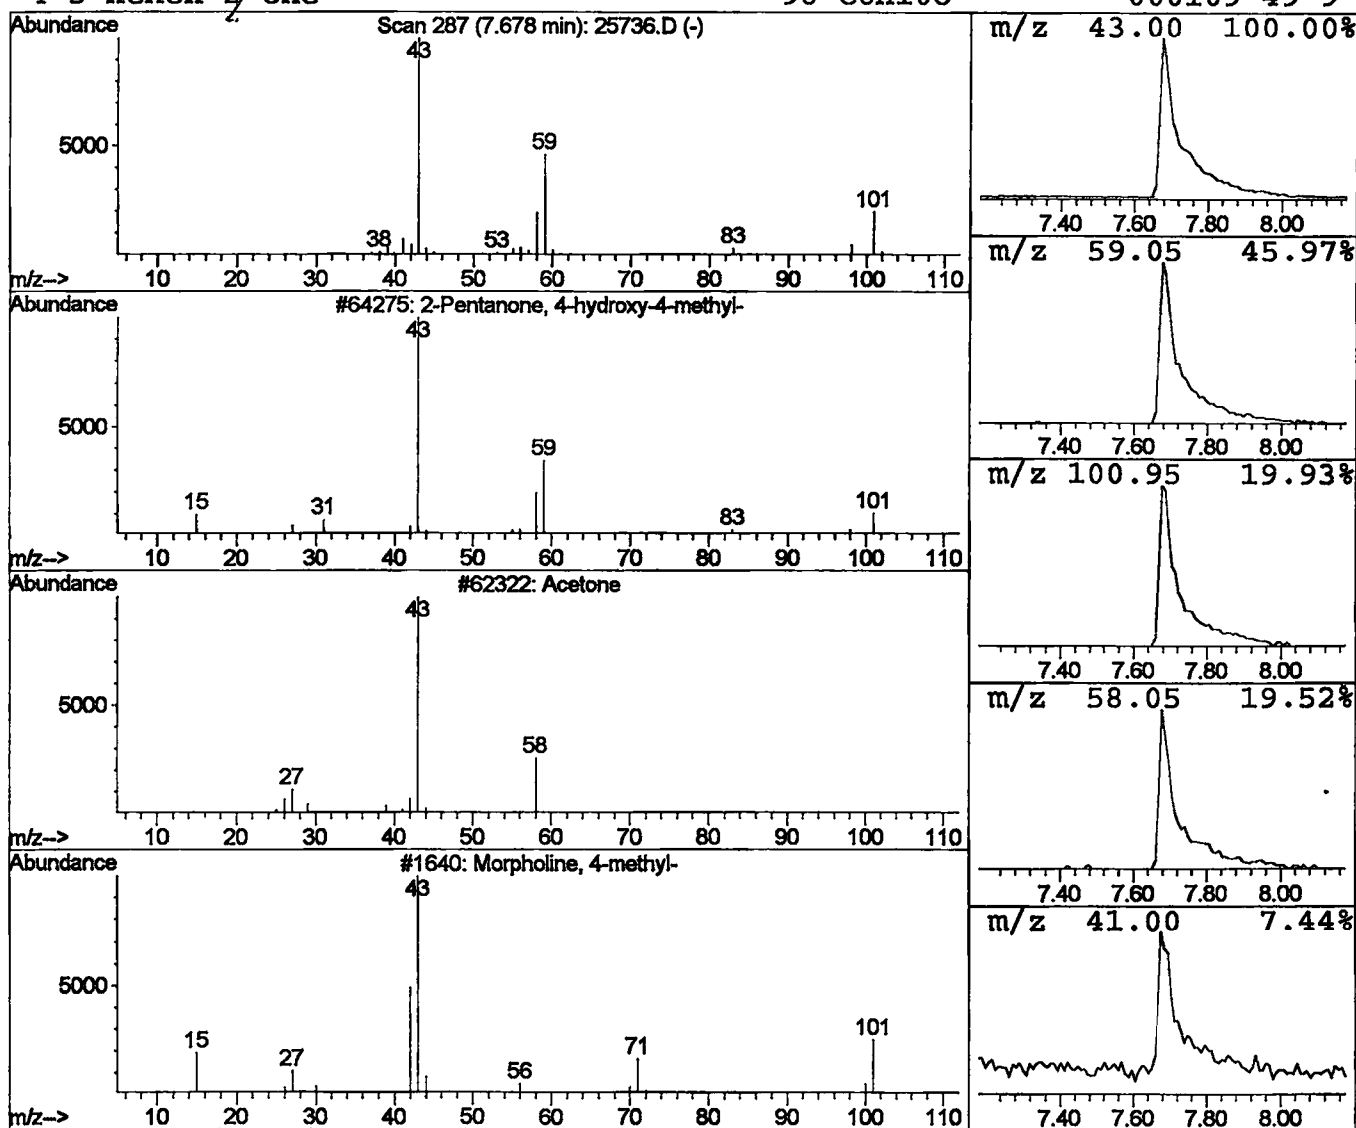

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 17 Nov 2001 12:30 pm
 Data File: C:\HPCHEM\1\DATA\NOV1601\25736.D
 Name: gc/ms unknown
 Misc:
 Method: C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc Units	Area	IntStd	ISRT	ISArea	ISConc
-----	-----	-----	-----	-----	-----	-----	-----
2-Hexanone	6.41	0.4 ug/l	68536	ISTD01	11.71	3209400	20.0
2-Pentanone, 4-hydro	7.68	2.4 ug/l	389971	ISTD01	11.71	3209400	20.0

25736.D NP103001.M Thu Nov 29 09:21:28 2001