

User: Galos, Marie
 Westchester Dept. of Labs & Research
 Date: 12/06/2001 Time: 15:50:08

Sample: AD25843
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 12/6/01 15:49 Ended: 12/6/01 15:49 Analyst: MG
 Page: 1

Component Name	Qty	Result
Other unknown compounds		see comment

Comments for Sample AD25843 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Galos, Marie

Date: 12-06-2001 Time: 15:50:12

A scan of the extract prepared for the 508 analysis, from 35-550 amu using a mass spectrometer, does not reveal the presence of non-target compounds.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV1901\25843.D

Vial: 10

Acq On : 20 Nov 2001 12:05 am

Operator: 209 GALOS

Sample : gc/ms unknown

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Nov 20 0:53 2001

Quant Results File: NP103001.RES

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Nov 02 16:41:16 2001

Response via : Initial Calibration

DataAcq Meth : NP103001

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	11.72	152	693792	20.00	ug/l	0.00
19) Naphthalene-d8	15.31	136	2700731	20.00	ug/l	-0.02
31) Acenaphthene-d10	20.59	164	1362087	20.00	ug/l	-0.02
49) Phenanthrene-d10	25.02	188	2029626	20.00	ug/l	-0.02
59) Chrysene-d12	33.05	240	1508332	20.00	ug/l	-0.02
68) Perylene-d12	37.15	264	1114253	20.00	ug/l	0.00

System Monitoring Compounds

4) 2-Fluorophenol	0.00	112	0	0.00	ug/l	
Spiked Amount	75.000		Recovery	=	0.00%	
5) Phenol-d5	0.00	99	0	0.00	ug/l	
Spiked Amount	75.000		Recovery	=	0.00%	
6) 2-Chlorophenol-d4	11.71	132	405	0.01	ug/l	0.47
Spiked Amount	75.000		Recovery	=	0.01%	
7) 1,2-Dichlorobenzene-d4	12.27	152	880	0.03	ug/l	0.02
Spiked Amount	50.000		Recovery	=	0.06%	
20) Nitrobenzene-d5	0.00	82	0	0.00	ug/l	
Spiked Amount	50.000		Recovery	=	0.00%	
32) 2-Fluorobiphenyl	18.75	172	2034	0.02	ug/l	0.13
Spiked Amount	50.000		Recovery	=	0.04%	
33) 2,4,6-Tribromophenol	0.00	330	0	0.00	ug/l	
Spiked Amount	75.000		Recovery	=	0.00%	
62) Terphenyl-d14	0.00	244	0	0.00	ug/l	
Spiked Amount	50.000		Recovery	=	0.00%	

Target Compounds

					Qvalue
2) Pyridine	0.00	79	0	N.D.	
3) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
8) Phenol	0.00	94	0	N.D.	
9) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
10) 2-Chlorophenol	0.00	128	0	N.D.	
11) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
12) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
13) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
14) 2-Methylphenol	0.00	108	0	N.D.	
15) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
16) 3&4-Methylphenol	0.00	108	0	N.D.	
17) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
18) Hexachloroethane	0.00	117	0	N.D.	
21) Nitrobenzene	0.00	77	0	N.D.	
22) Isophorone	0.00	82	0	N.D.	

(#)=qualifier out of range (m)=manual integration

25843.D NP103001.M Wed Dec 05 15:15:51 2001

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV1901\25843.D
 Acq On : 20 Nov 2001 12:05 am
 Sample : gc/ms unknown
 Misc :
 MS Integration Params: RTEINT.P
 Quant Time: Nov 20 0:53 2001

Vial: 10
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: NP103001.RES

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Fri Nov 02 16:41:16 2001
 Response via : Initial Calibration
 DataAcq Meth : NP103001

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
23) 2-Nitrophenol	0.00	139	0	N.D.		
24) 2,4-Dimethylphenol	0.00	107	0	N.D.		
25) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.		
26) 2,4-Dichlorophenol	0.00	162	0	N.D.		
27) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.		
28) Naphthalene	15.38	128	824	N.D.		
29) Hexachlorobutadiene	0.00	225	0	N.D.		
30) 4-Chloro-3-methylphenol	0.00	107	0	N.D.		
34) Hexachlorocyclopentadiene	0.00	237	0	N.D.		
35) 2,4,6-Trichlorophenol	0.00	196	0	N.D.		
36) 2,4,5-Trichlorophenol	0.00	196	0	N.D.		
37) 2-Chloronaphthalene	0.00	162	0	N.D.		
38) Dimethylphthalate	0.00	163	0	N.D.		
39) 2,6-Dinitrotoluene	0.00	165	0	N.D.		
40) Acenaphthylene	0.00	152	0	N.D.		
41) Acenaphthene	0.00	153	0	N.D.		
42) 2,4-Dinitrophenol	0.00	184	0	N.D.		
43) 4-Nitrophenol	0.00	65	0	N.D.		
44) 2,4-Dinitrotoluene	20.87	165	216	N.D.		
45) Diethylphthalate	0.00	149	0	N.D.		
46) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.		
47) Fluorene	0.00	166	0	N.D.		
48) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.		
50) 4,6-Dinitro-2-methylphenol	0.00	198	0	N.D.		
51) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
52) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
53) Hexachlorobenzene	0.00	284	0	N.D.		
54) Pentachlorophenol	0.00	266	0	N.D.		
55) Phenanthrene	25.08	178	206	N.D.		
56) Anthracene	25.08	178	206	N.D.		
57) Di-n-butylphthalate	27.05	149	2241	N.D.		
58) Fluoranthene	0.00	202	0	N.D.		
60) 3,3'-Dichlorobenzidine	0.00	252	0	N.D.		
61) Benzidine	0.00	184	0	N.D.		
63) Pyrene	0.00	202	0	N.D.		
64) Butylbenzylphthalate	0.00	149	0	N.D.		
65) Benzo(a)anthracene	33.05	228	3587	N.D.		
66) Bis(2-ethylhexyl)phthalate	33.33	149	1278	N.D.		
67) Chrysene	33.05	228	3587	N.D.		
69) Di-n-Octylphthalate	0.00	149	0	N.D.		
70) Benzo(b)fluoranthene	0.00	252	0	N.D.		

(#) = qualifier out of range (m) = manual integration

25843.D NP103001.M Wed Dec 05 15:15:56 2001

Page 2

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV1901\25843.D

Vial: 10

Acq On : 20 Nov 2001 12:05 am

Operator: 209 GALOS

Sample : gc/ms unknown

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Nov 20 0:53 2001

Quant Results File: NP103001.RES

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Nov 02 16:41:16 2001

Response via : Initial Calibration

DataAcq Meth : NP103001

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
71) Benzo(k)fluoranthene	0.00	252	0	N.D.		
72) Benzo(a)pyrene	37.15	252	4200	N.D.		
73) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
74) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
75) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

25843.D NP103001.M Wed Dec 05 15:15:57 2001

Page 3


Quantitation Report

Data File : C:\HPCHEM\1\DATA\NOV1901\25843.D
Acq On : 20 Nov 2001 12:05 am
Sample : gc/ms unknown
Misc :
MS Integration Params: RTEINT.P
Quant Time: Nov 20 0:53 2001

Vial: 10
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: NP103001.RES

Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Fri Nov 02 16:41:16 2001
Response via : Initial Calibration

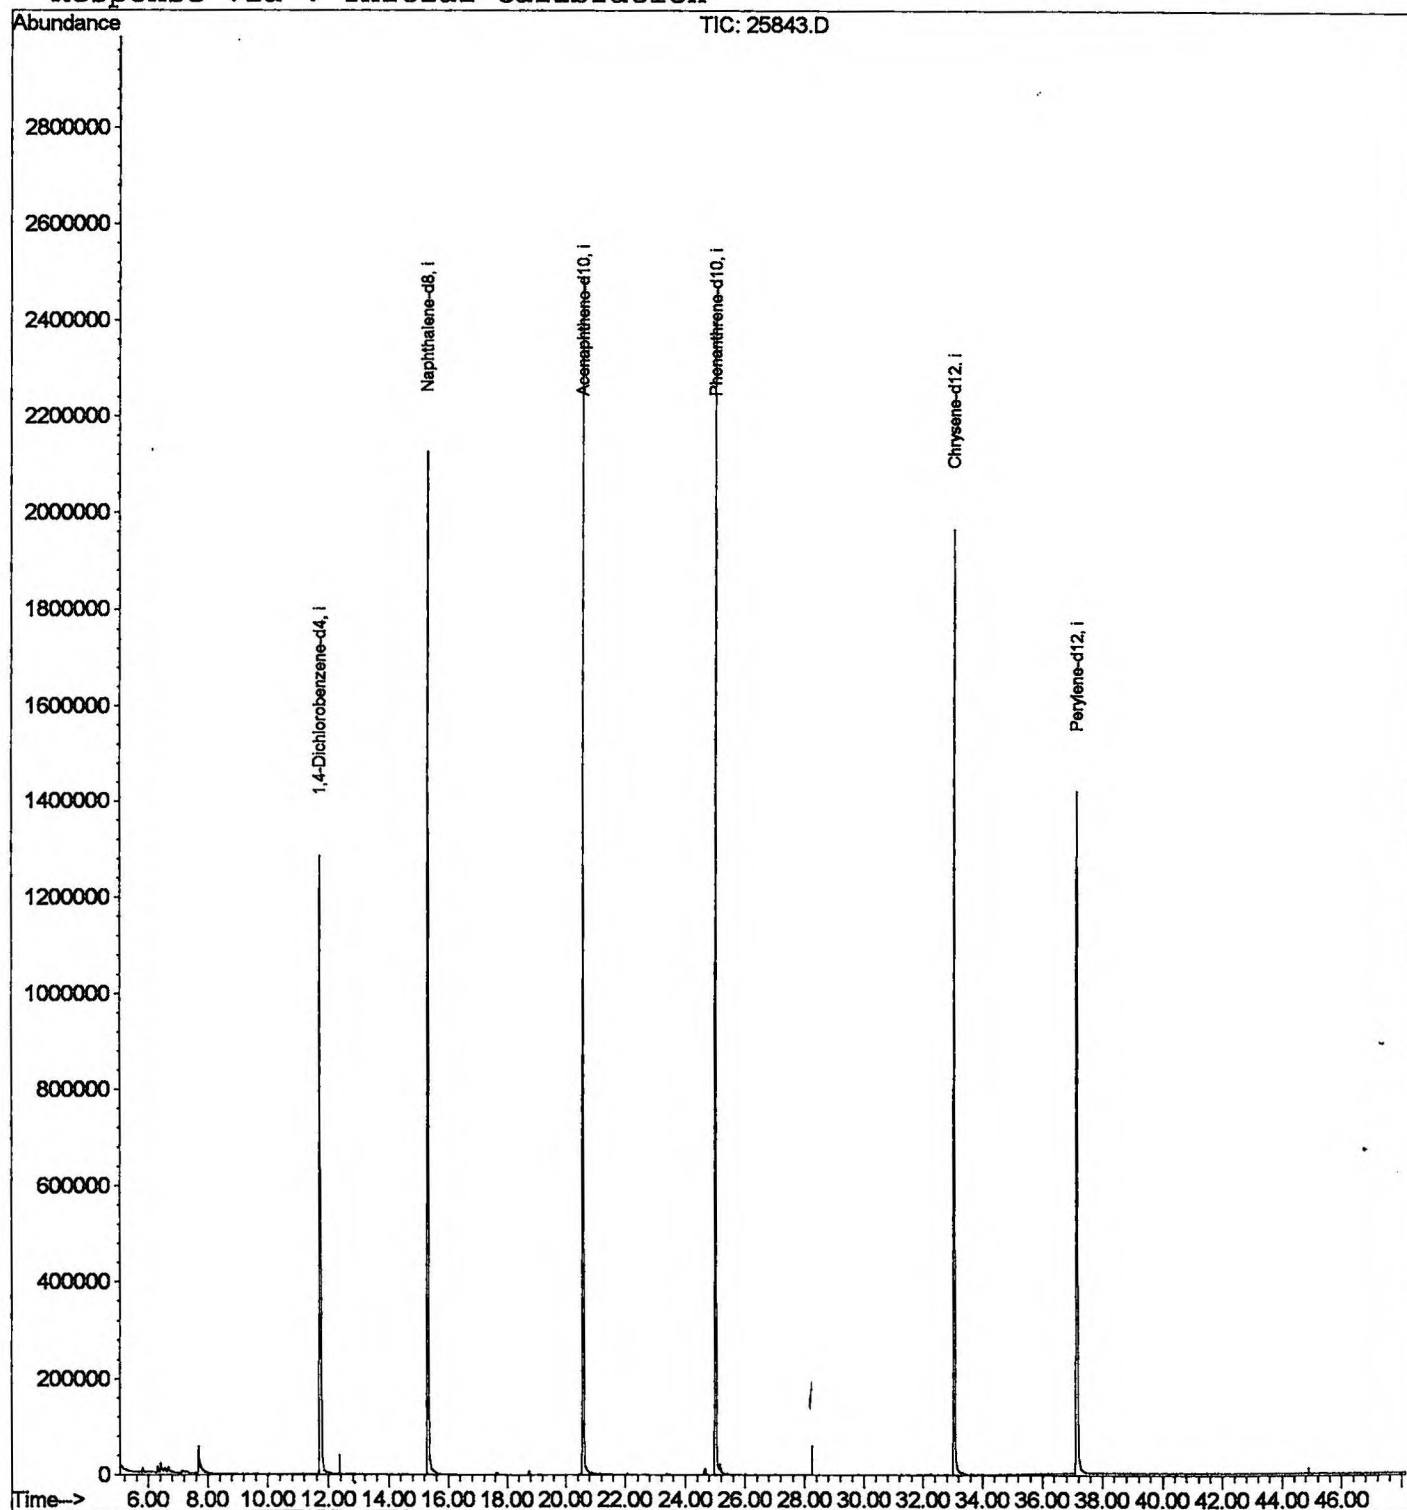

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\NOV1901\25843.D
 Acq On : 20 Nov 2001 12:05 am
 Sample : gc/ms unknown
 Misc :
 MS Integration Params: LSCINT.P

Vial: 10
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC




peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	7.694	285	289	306	rBV	56729	218887	4.00%	0.770%
2	11.715	721	727	750	rBV	1285527	3619748	66.12%	12.734%
3	15.314	1114	1119	1138	rBV	2125267	4907597	89.64%	17.264%
4	20.593	1688	1694	1714	rBV	2490674	5474561	100.00%	19.259%
5	25.017	2170	2176	2188	rBV2	2404840	5295245	96.72%	18.628%
6	25.164	2188	2192	2206	rVB2	19984	66003	1.21%	0.232%
7	33.050	3044	3051	3065	rBV2	1965633	4711610	86.06%	16.575%
8	37.154	3489	3498	3517	rBV2	1419513	4132505	75.49%	14.538%

Sum of corrected areas: 28426156

25843.D NP103001.M Wed Dec 05 15:36:11 2001

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\NOV1901\25843.D
 Operator : 209 GALOS
 Acquired : 20 Nov 2001 12:05 am using AcqMethod NP103001
 Instrument : GC/MS 209
 Sample Name: gc/ms unknown
 Misc Info :
 Vial Number: 10
 Quant File :NP103001.RES (RTE Integrator)

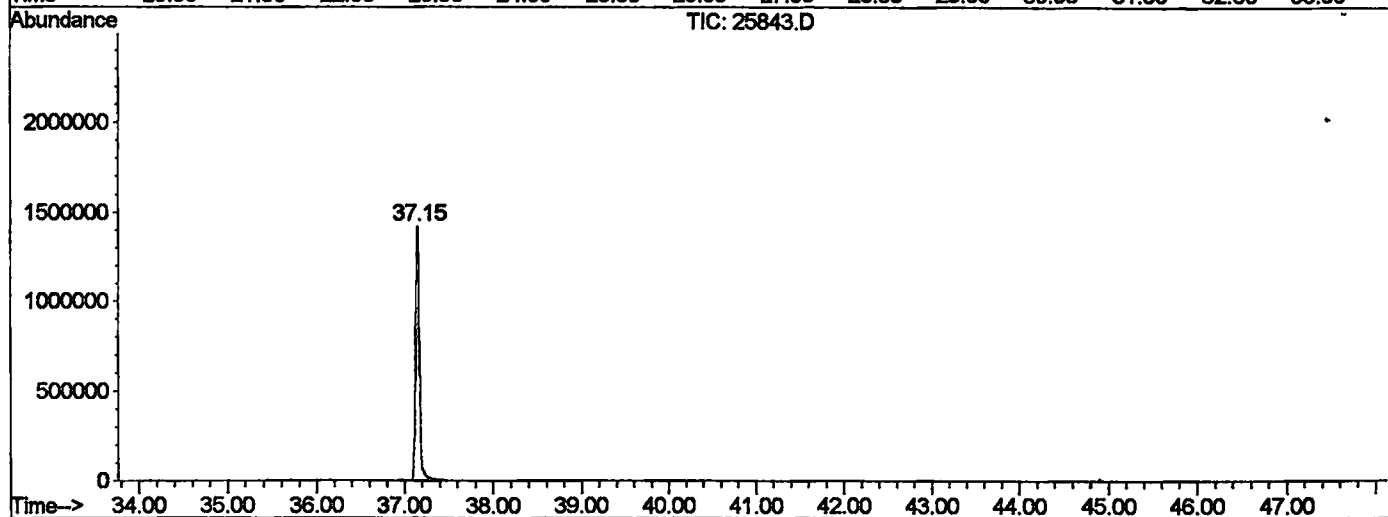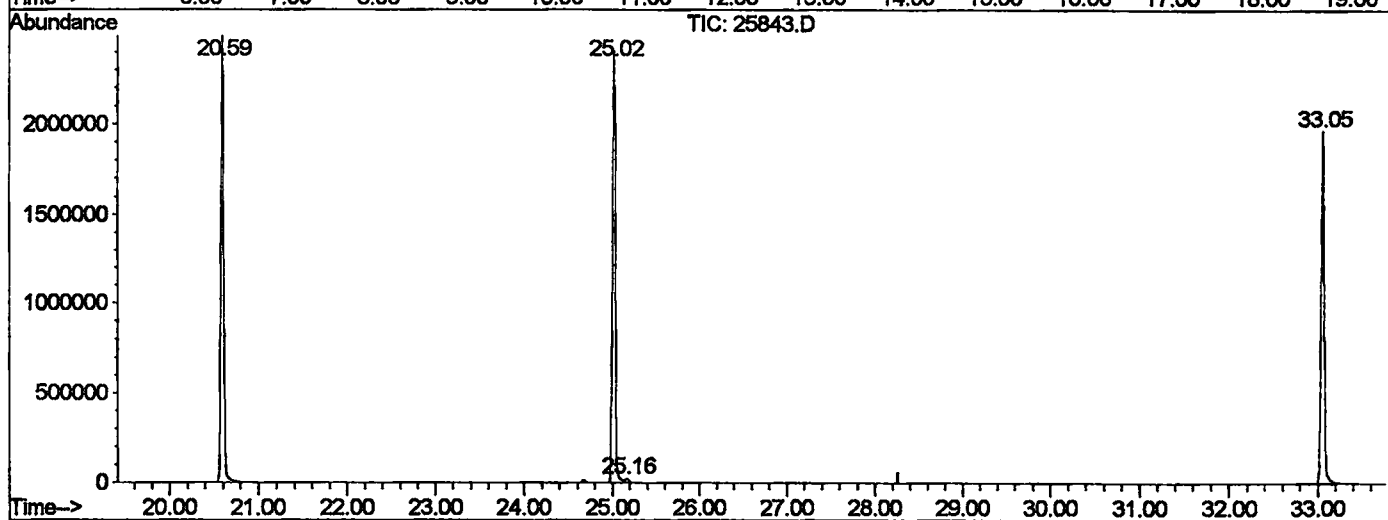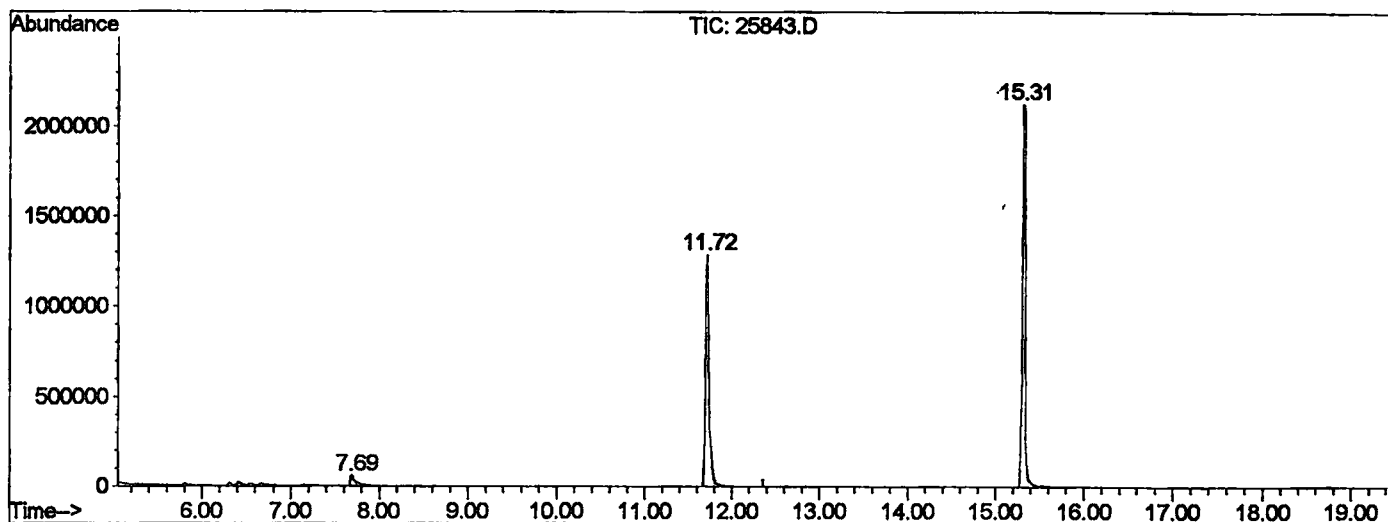

25843.D NP103001.M Wed Dec 05 15:36:13 2001

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\NOV1901\25843.D
Acq On : 20 Nov 2001 12:05 am
Sample : gc/ms unknown
Misc :
MS Integration Params: LSCINT.P










Vial: 10
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.69	1.21 ug/l	218887	1,4-Dichlorobenzene-d4	11.72

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	42		
2	5-Hexen-2-one	98	C6H10O	000109-49-9	9		
3	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9		
4	tert-Butyl Hydroperoxide	90	C4H10O2	000075-91-2	9		

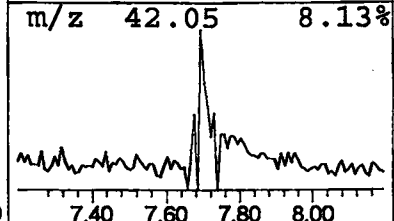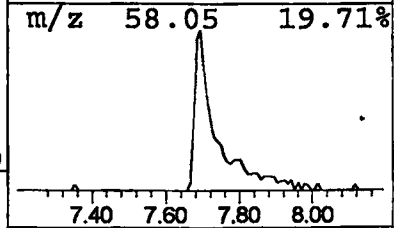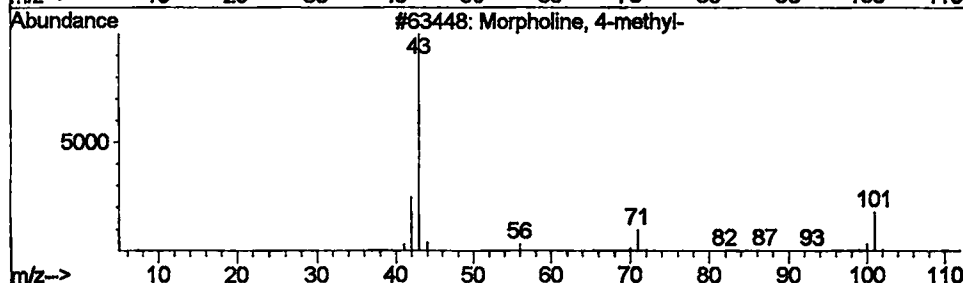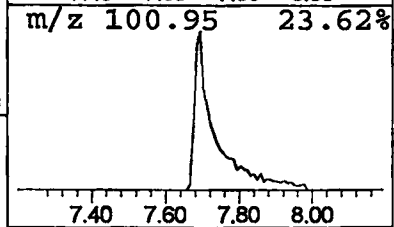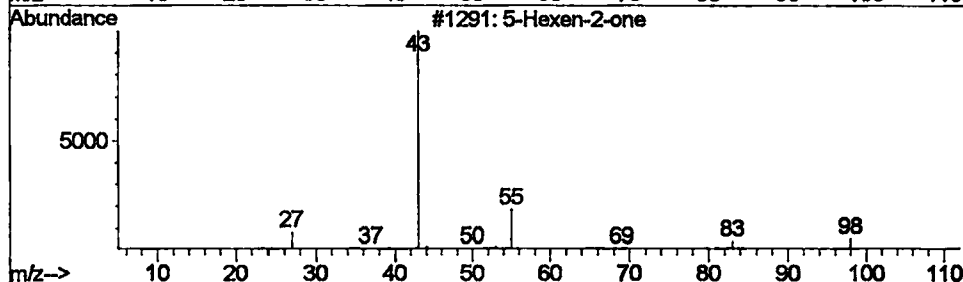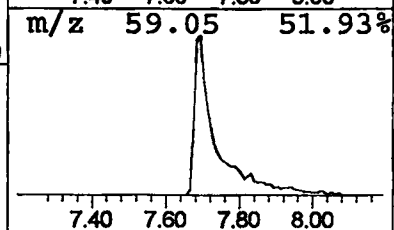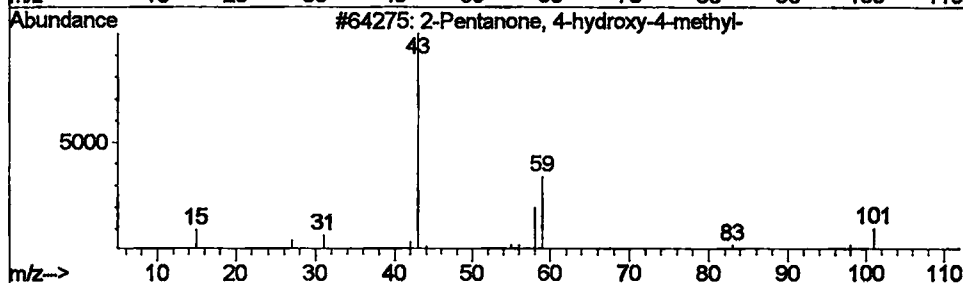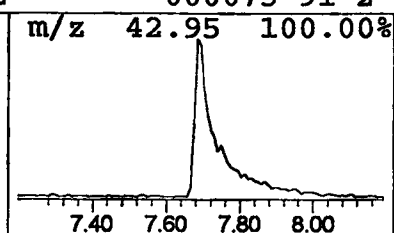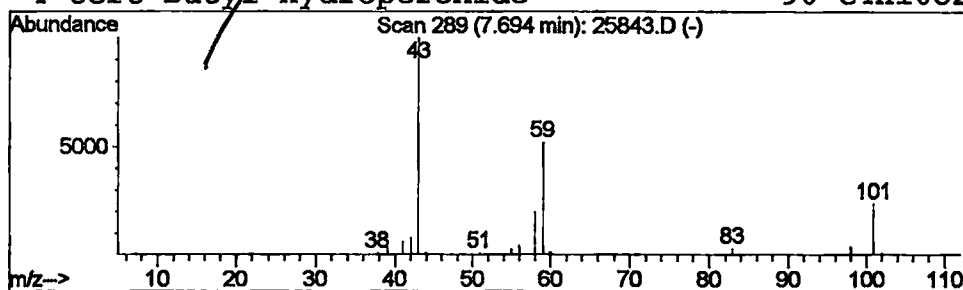

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 20 Nov 2001 12:05 am
Data File: C:\HPCHEM\1\DATA\NOV1901\25843.D
Name: gc/ms unknown
Misc:
Method: C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	7.69	1.2 ug/l		218887	ISTD01	11.72	3619750	20.0
25843.D NP103001.M								

Wed Dec 05 15:36:18 2001