

User: Nefliu, Marcela
Westchester Dept. of Labs & Research
Date: 10/17/2001 Time: 10:57:41

Sample: AD25441
Analysis: \$508 Chlorine Pesticides - 508
Units: ug
Started: 9/24/01 10:53 Ended: 10/2/01 10:53 Analyst: MN
Result source: manual entry
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Propachlor		< MDL		0.040
2	Lindane		< MDL		0.030
3	Heptachlor		< MDL		0.020
4	Aldrin		< MDL		0.010
5	Heptachlor Epoxide		< MDL		0.030
6	4,4-DDE		< MDL		0.080
7	Dieldrin		< MDL		0.016
8	Endrin		< MDL		0.020
9	Methoxychlor		< MDL		0.039
10	Chlordane		< MDL		0.40
11	Toxaphene		< MDL		0.40
12	PCB's		< MDL		0.20
13	Surr_2,4-DDD		0.13		

Not our sample
QC only
tap water

Faul

Quantitation Report (QT Reviewed)

Signal #1 : C:\HPCHEM\1\DATA\508F\011002B\TW.D\ECD1A.CH Vial: 56
 Signal #2 : C:\HPCHEM\1\DATA\508F\011002B\TW.D\ECD2B.CH
 Acq On : 3 Oct 2001 6:22 pm Operator: Nefliu
 Sample : tap water Inst : 104
 Misc : Multiplr: 1.00
 IntFile Signal #1: events.e IntFile Signal #2: events2.e
 Quant Time: Oct 9 15:36 2001 Quant Results File: 011002P.RES

Quant Method : C:\HPCHEM\1\METHODS\011002P.M (Chemstation Integrator)
 Title : 508 CHLORINATED PESTICIDES 9/6/00
 Last Update : Fri Sep 28 14:35:02 2001
 Response via : Initial Calibration
 DataAcq Meth : 508F.M

Volume Inj. :
 Signal #1 Phase : Signal #2 Phase:
 Signal #1 Info : Signal #2 Info :

Compound	RT#1	RT#2	Resp#1	Resp#2	ug/L	ug/L	

System Monitoring Compounds							
10) S 2,4-DDD SURROGAT	37.60	0.00	632578	0	0.133	N.D.	#
Spiked Amount 0.100			Recovery	=	133.00%	0.00%	
Target Compounds							
1) PROPACHLOR	17.47	0.00	1343	0	0.002	N.D.	#
2) g-BHC	23.83	0.00	19141	0	0.002	N.D.	#
3) HEPTACHLOR	26.45	0.00	954	0	0.000	N.D.	#
4) ALDRIN	28.78	0.00	1319	0	0.000	N.D.	#
5) HEPTACHLOR EPOXI	32.58	0.00	3729	0	0.000	N.D.	#
6) 4,4'-DDE	36.08	0.00	33262	0	0.004	N.D.	#
7) DIELDRIN	36.56	33.98	8217	893	0.001	0.000	#
8) ENDRIN	38.70	0.00	705	0	0.000	N.D.	#


 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.
 TW.D 011002P.M Wed Oct 17 10:28:17 2001

Quantitation Report

Signal #1 : C:\HPCHEM\1\DATA\508F\011002B\TW.D\ECD1A.CH Vial: 56
Signal #2 : C:\HPCHEM\1\DATA\508F\011002B\TW.D\ECD2B.CH
Acq On : 3 Oct 2001 6:22 pm Operator: Nefliu
Sample : tap water Inst : 104
Misc : Multiplr: 1.00
IntFile Signal #1: events.e IntFile Signal #2: events2.e
Quant Time: Oct 9 15:36 2001 Quant Results File: 011002P.RES

Quant Method : C:\HPCHEM\1\METHODS\011002P.M (Chemstation Integrator)
Title : 508 CHLORINATED PESTICIDES 9/6/00
Last Update : Fri Sep 28 14:35:02 2001
Response via : Multiple Level Calibration
DataAcq Meth : 508F.M

Volume Inj. :
Signal #1 Phase :
Signal #1 Info :
Signal #2 Phase :
Signal #2 Info :

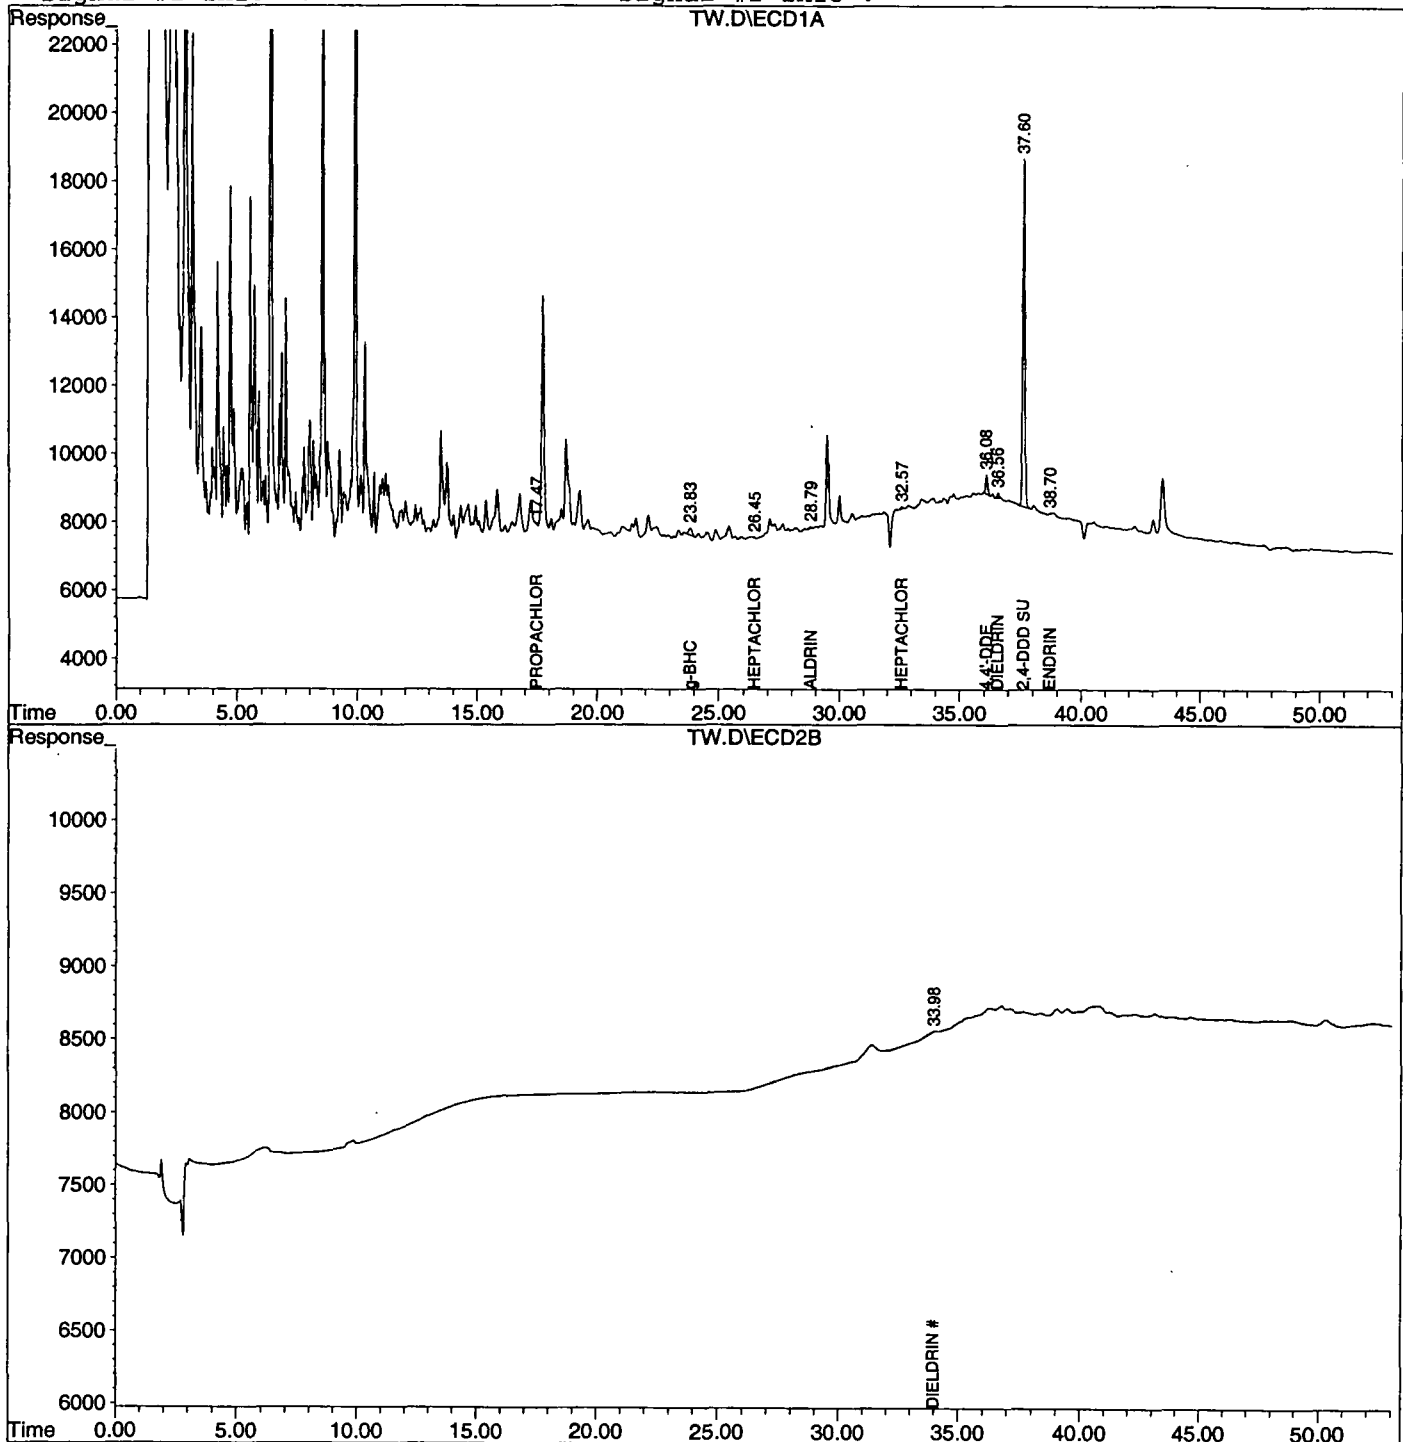

Quantitation Report (QT Reviewed)

Signal #1 : C:\HPCHEM\1\DATA\508F\011002B\TW.D\ECD1A.CH Vial: 56
Signal #2 : C:\HPCHEM\1\DATA\508F\011002B\TW.D\ECD2B.CH
Acq On : 3 Oct 2001 6:22 pm Operator: Nefliu
Sample : tap water Inst : 104
Misc : Multiplr: 1.00
IntFile Signal #1: events.e IntFile Signal #2: events2.e
Quant Time: Oct 17 10:29 2001 Quant Results File: 010828C.RES

Quant Method : C:\HPCHEM\1\METHODS\010828C.M (Chemstation Integrator)
Title : DUAL 508 CHLORINATED PESTICIDES CHLORDANE 6/3/99
Last Update : Sun Sep 30 10:30:23 2001
Response via : Initial Calibration
DataAcq Meth : 508F.M

Volume Inj. :
Signal #1 Phase : Signal #2 Phase:
Signal #1 Info : Signal #2 Info :

Compound	RT#1	RT#2	Resp#1	Resp#2	ug/L	ug/L
System Monitoring Compounds						
4) s 2,4-DDD SURROGAT	37.60	0.00	629493	0	0.138m	N.D. #
Spiked Amount 0.100			Recovery	=	138.00%	0.00%
Target Compounds						
3) CHLORDANE PEAK 3	34.73	0.00	5952	0	0.008	N.D. #

Quantitation Report

Signal #1 : C:\HPCHEM\1\DATA\508F\011002B\TW.D\ECD1A.CH Vial: 56
Signal #2 : C:\HPCHEM\1\DATA\508F\011002B\TW.D\ECD2B.CH
Acq On : 3 Oct 2001 6:22 pm Operator: Nefliu
Sample : tap water Inst : 104
Misc : Multiplr: 1.00
IntFile Signal #1: events.e IntFile Signal #2: events2.e
Quant Time: Oct 17 10:29 2001 Quant Results File: 010828C.RES

Quant Method : C:\HPCHEM\1\METHODS\010828C.M (Chemstation Integrator)
Title : DUAL 508 CHLORINATED PESTICIDES CHLORDANE 6/3/99
Last Update : Sun Sep 30 10:30:23 2001
Response via : Multiple Level Calibration
DataAcq Meth : 508F.M

Volume Inj. :
Signal #1 Phase : Signal #2 Phase:
Signal #1 Info : Signal #2 Info :

