



User: Bohlk, Ted
Westchester Dept. of Labs & Research
Date: 05/03/2002 Time: 14:48:41

Sample: AE10186
Analysis: SLP525 Organic Extractables
Units: ug
Started: 5/2/02 14:47 Ended: 5/2/02 14:47 Analyst: TB
Page: 1

	Component Name	Viol	Result
1	DFTPP		PASSED
2	ENDRIN		7.2
3	DDT		0



File : C:\MSDCHEM\1\DATA\050202\DFTA0502.D
 Operator : Bohlk / Inst 213
 Acquired : 2 May 2002 12:25 pm using AcqMethod 050102
 Instrument : Instrumen
 Sample Name: DFTPP/ENDRIN
 Misc Info :
 Vial Number: 1

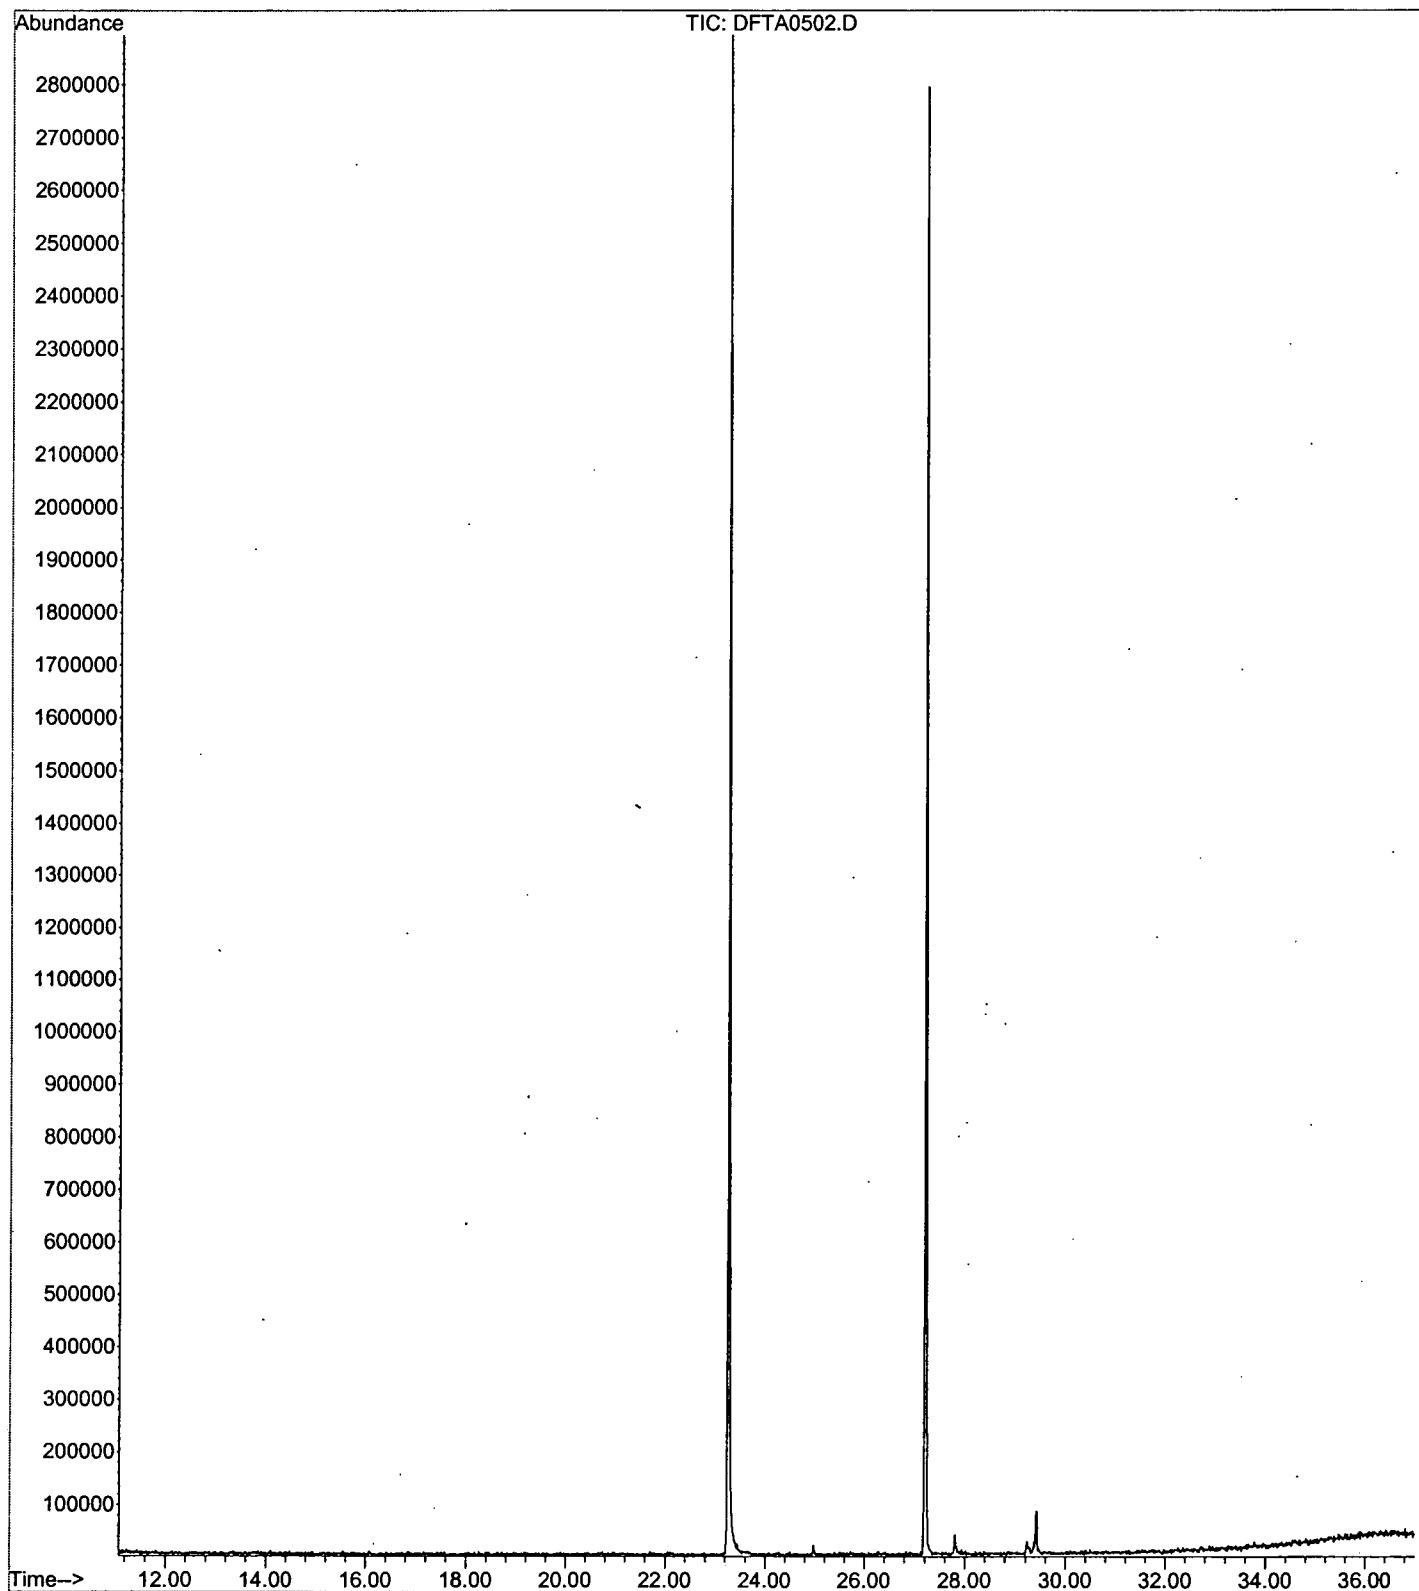

DFTPP

Data File : C:\MSDCHEM\1\DATA\050202\DFTA0502.D
Acq On : 2 May 2002 12:25 pm
Sample : DFTPP/ENDRIN
Misc :
MS Integration Params: rteint.p

Vial: 1
Operator: Bohlk / Inst 213
Inst : Instrumen
Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\050102.M (RTE Integrator)
Title : Quantitation For Method 525.2

Spectrum Information: Average of 23.194 to 23.402 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.2	19094	PASS
68	69	0.00	2	1.5	334	PASS
69	198	0.00	100	42.3	22991	PASS
70	69	0.00	2	0.3	74	PASS
127	198	10	80	56.3	30569	PASS
197	198	0.00	2	0.4	202	PASS
198	198	50	100	100.0	54290	PASS
199	198	5	9	6.6	3586	PASS
275	198	10	60	18.8	10218	PASS
365	198	1	100	2.1	1116	PASS
441	443	0.01	100	73.0	4977	PASS
442	198	50	100	65.0	35290	PASS
443	442	15	24	19.3	6815	PASS

DFTA0502.D 050102.M Thu May 02 15:31:09 2002

Area Percent Report

Data File : C:\MSDCHEM\1\DATA\050202\DFTA0502.D
 Acq On : 2 May 2002 12:25 pm
 Sample : DFTPP/ENDRIN
 Misc :
 MS Integration Params: rteint.p

Vial: 1
 Operator: Bohlk / Inst 213
 Inst : Instrumen
 Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\050102.M (RTE Integrator)
 Title : Quantitation For Method 525.2
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 5000 Area counts
 Start Thrs: 0.2 Max Peaks: 10
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC


peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	27.212	1773	1779	1786	rM 2	2794133	5466842	100.00%	92.806%
2	27.811	1842	1845	1851	rM 5	34623	74823	1.37%	1.270%
3	29.425	1999	2023	2032	rM 5	81951	348943	6.38%	5.924%

> 7.2%

Sum of corrected areas: 5890608

Endrin
 Breakdown

File : C:\MSDCHEM\1\DATA\050202\DDTA0502.D
Operator : Bohlk / Inst 213
Acquired : 2 May 2002 1:17 pm using AcqMethod 050102
Instrument : Instrumen
Sample Name: DDT
Misc Info :
Vial Number: 2

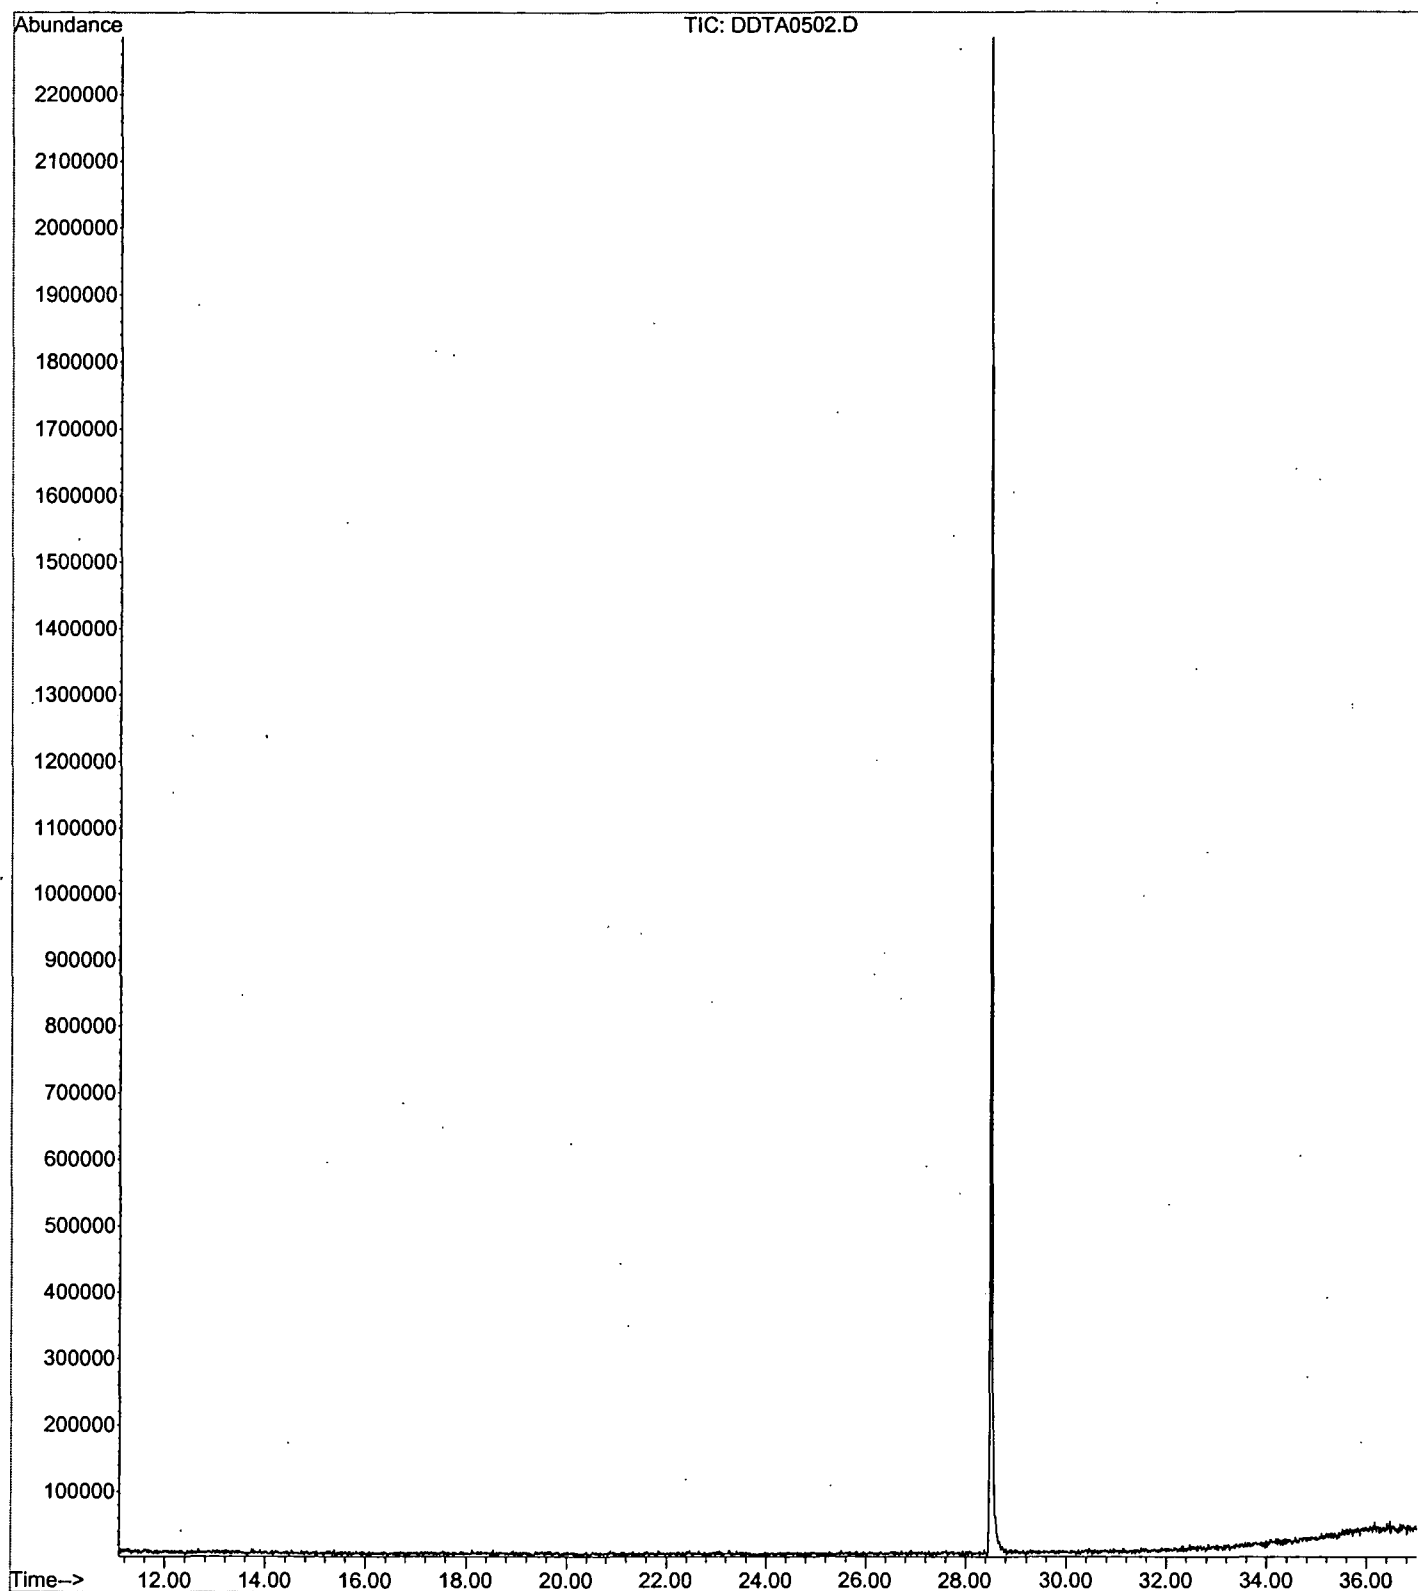

Area Percent Report

Data File : C:\MSDCHEM\1\DATA\050202\DDTA0502.D
Acq On : 2 May 2002 1:17 pm
Sample : DDT
Misc :
MS Integration Params: rteint.p

Vial: 2
Operator: Bohlk / Inst 213
Inst : Instrumen
Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\050102.M (RTE Integrator)
Title : Quantitation For Method 525.2
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 5000 Area counts
Start Thrs: 0.2 Max Peaks: 10
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	28.491	1913	1920	1955	rM	2281023	5084762	100.00%	100.000%

Sum of corrected areas: 5084762