

Sequence Name: C:\HPCHEM\1\SEQUENCE\SEP2101.S

Comment: 208

Operator: GALOS

Data Path: C:\HPCHEM\1\DATA\sep2101\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run

On A Barcode Mismatch

☒ Full Method☒ Inject Anyway☐ Reprocessing Only☐ Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	HP060501	
2	Sample	2	22470	HP060501	GC/MS unknown
3	Sample	3	22471	HP060501	GC/MS unknown
4	Sample	4	22472	HP060501	GC/MS unknown
5	Sample	5	22485	HP060501	GC/MS unknown
6	Sample	6	22486	HP060501	GC/MS unknown
7	Sample	7	22487	HP060501	GC/MS unknown
8	Sample	8	22488	HP060501	GC/MS unknown
9	Sample	9	22489	HP060501	GC/MS unknown

DFTPP

Data File : C:\HPCHEM\1\DATA\SEP2101\DFTPP.D

Acq On : 21 Sep 2001 12:33 pm

Sample :

Misc :

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\NY082801.M (RTE Integrator)


Title : 208 1 scan method NEW YORK PESTICIDES

Vial: 1

Operator: GALOS

Inst : GC/MS Ins

Multiplr: 1.00

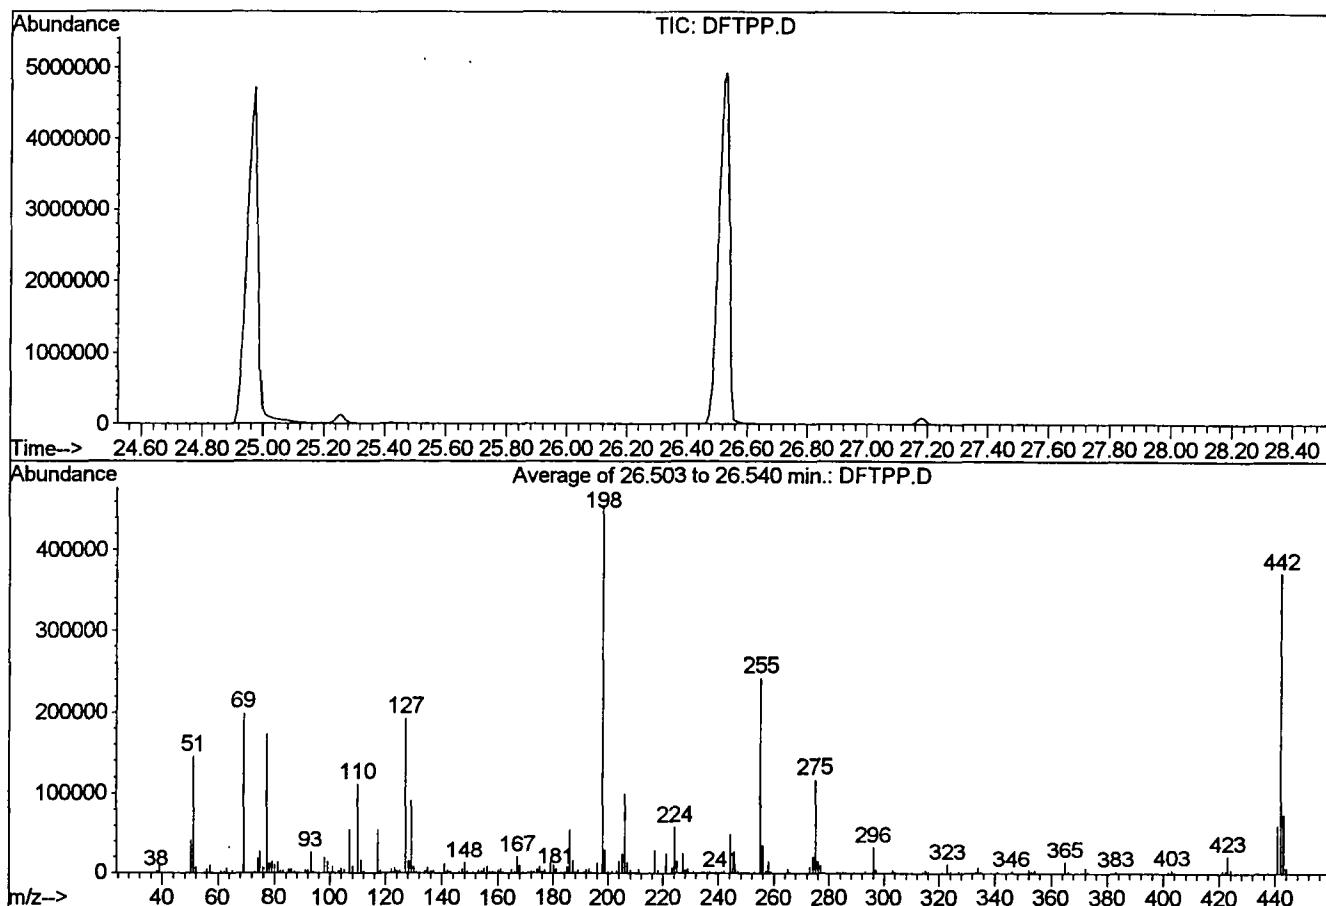

Spectrum Information: Average of 26.503 to 26.540 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	32.0	145251	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.8	198872	PASS
70	69	0.00	2	0.4	825	PASS
127	198	40	60	42.4	192774	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	454387	PASS
199	198	5	9	6.6	30176	PASS
275	198	10	30	25.8	117355	PASS
365	198	1	99	3.0	13635	PASS
441	443	1	99	81.6	60653	PASS
442	198	40	110	81.7	371123	PASS
443	442	17	23	20.0	74342	PASS

DFTPP.D NY082801.M

Fri Sep 21 15:24:01 2001