

Method 508 Date Extracted 9/17/01 Page 83
5 cells

[illegible]

Sequence Name: C:\HPCHEM\1\SEQUENCE\SEP2501.S
Comment: INST 209; 30Mx0.25umX0.50
Operator: 209 GALOS
Data Path: C:\HPCHEM\1\data\sep2501\
Pre-Seq Cmd:
Post-Seq Cmd:


Method Sections To Run On A Barcode Mismatch
(X) Full Method (X) Inject Anyway
() Reprocessing Only () Don't Inject

Line Type	Vial	DataFile	Method	Sample Name
1 Sample	1	DFTPP	NP091101	
2 Sample	2	22491 ✓	NP091101	GC/MS unknown
3 Sample	3	22492 ✓	NP091101	GC/MS unknown
4 Sample	4	22493 ✓	NP091101	GC/MS unknown
5 Sample	5	22494	NP091101	GC/MS unknown
6 Sample	6	22495 ✓	NP091101	GC/MS unknown
7 Sample	7	22496 ✓	NP091101	GC/MS unknown
8 Sample	8	22542 ✓	NP091101	GC/MS unknown
9 Sample	9	22543 ✓	NP091101	GC/MS unknown
10 Sample	10	22544 ✓	NP091101	GC/MS unknown
11 Sample	11	22545 ✓	NP091101	GC/MS unknown
12 Sample	12	22546 ✓	NP091101	GC/MS unknown
13 Sample	13	22547 ✓	NP091101	GC/MS unknown

DFTPP

Data File : C:\HPCHEM\1\DATA\SEP2501\DFTPP.D
 Acq On : 25 Sep 2001 2:26 pm
 Sample :
 Misc :
 MS Integration Params: RTEINT.P
 Method : C:\HPCHEM\1\METHODS\NP091101.M (RTE Integrator)
 Title : 209 625/TCLP calibration table 7/16/01

Vial: 1
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

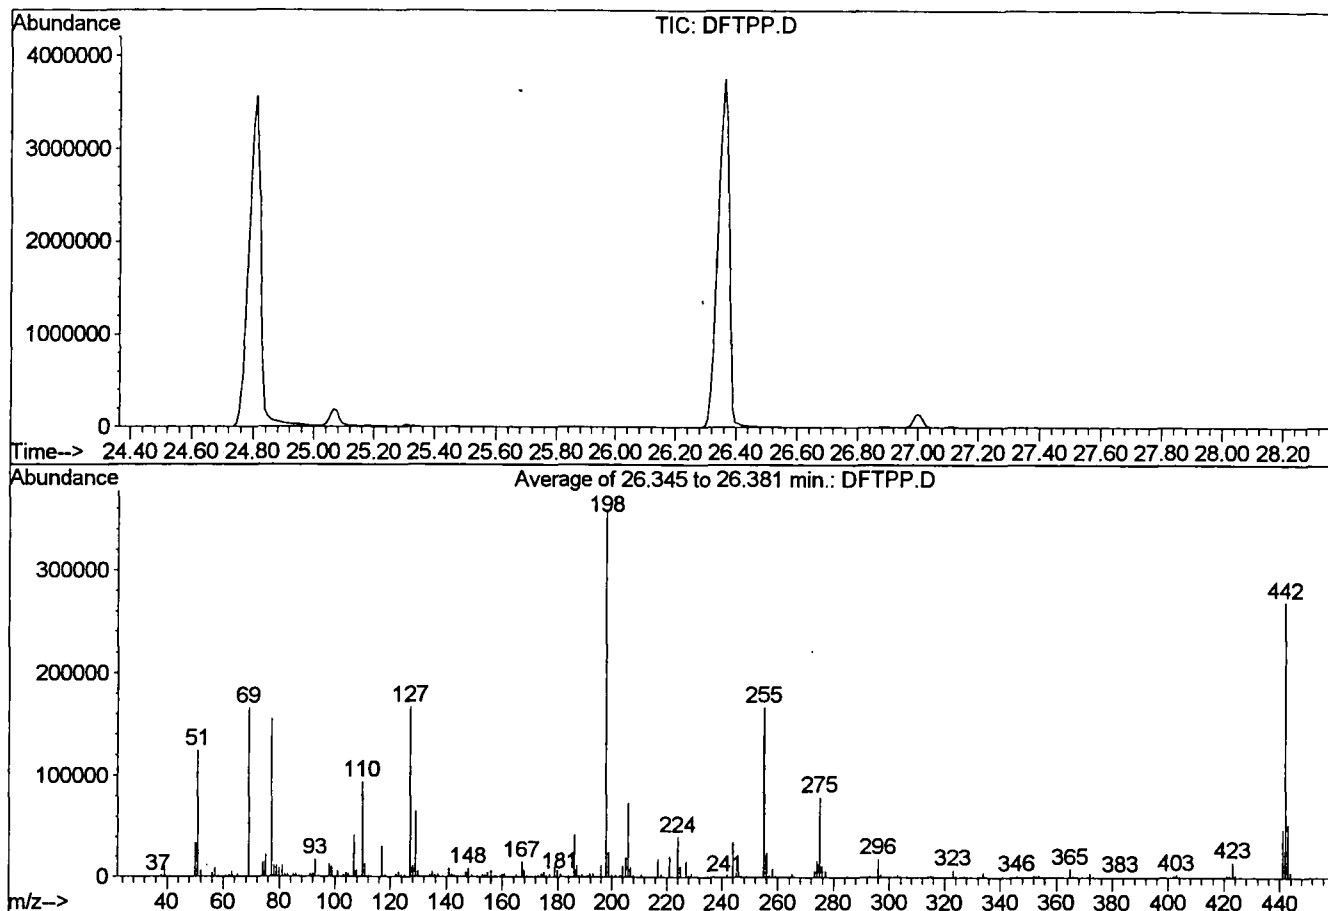

Spectrum Information: Average of 26.345 to 26.381 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	34.6	124424	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.0	165414	PASS
70	69	0.00	2	0.1	92	PASS
127	198	40	60	46.5	166976	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	359309	PASS
199	198	5	9	6.6	23737	PASS
275	198	10	30	22.1	79346	PASS
365	198	1	100	2.3	8144	PASS
441	443	0.01	100	89.8	46587	PASS
442	198	40	110	75.0	269517	PASS
443	442	17	23	19.3	51906	PASS