

Sequence Name: C:\HPCHEM\1\SEQUENCE\SEP2601.S
Comment: 208
Operator: GALOS
Data Path: C:\HPCHEM\1\DATA\sep2601\
Pre-Seq Cmd:
Post-Seq Cmd:

Method Sections To Run On A Barcode Mismatch
(X) Full Method (X) Inject Anyway
() Reprocessing Only () Don't Inject

Line Type	Vial	DataFile	Method	Sample Name
1 Sample	1	DFTPP	HP060501	
2 Sample	2	22548	HP060501	GC/MS unknown
3 Sample	3	22549	HP060501	GC/MS unknown
4 Sample	4	22550	HP060501	GC/MS unknown
5 Sample	5	22551	HP060501	GC/MS unknown
6 Sample	6	22552	HP060501	GC/MS unknown
7 Sample	7	22553	HP060501	GC/MS unknown
8 Sample	8	22577	HP060501	GC/MS unknown
9 Sample	9	22578	HP060501	GC/MS unknown

*do not
run
wrong vials*

Sequence Name: C:\HPCHEM\1\SEQUENCE\SEP2701.S

Comment: 208

Operator: GALOS

Data Path: C:\HPCHEM\1\DATA\sep2701\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run

On A Barcode Mismatch

☒ Full Method☒ Inject Anyway☐ Reprocessing Only☐ Don't Inject

Line Type	Vial	DataFile	Method	Sample Name
1 Sample	1	DFTPP	HP060501	
2 Sample	8	22577	HP060501	gc/ms unknown
3 Sample	9	22578	HP060501	gc/ms unknown
4 Sample	2	22558	HP060501	gc/ms unknown <1 ml
5 Sample	3	22577A	HP060501	gc/ms unknown <1 ml

Wrong line

DFTPP

Data File : C:\HPCHEM\1\DATA\OCT0101\DFTPP.D

Acq On : 1 Oct 2001 1:13 pm

Sample :


Misc :

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\NP091101.M (RTE Integrator)

Title : 209 625/TCLP calibration table 7/16/01

Vial: 1
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

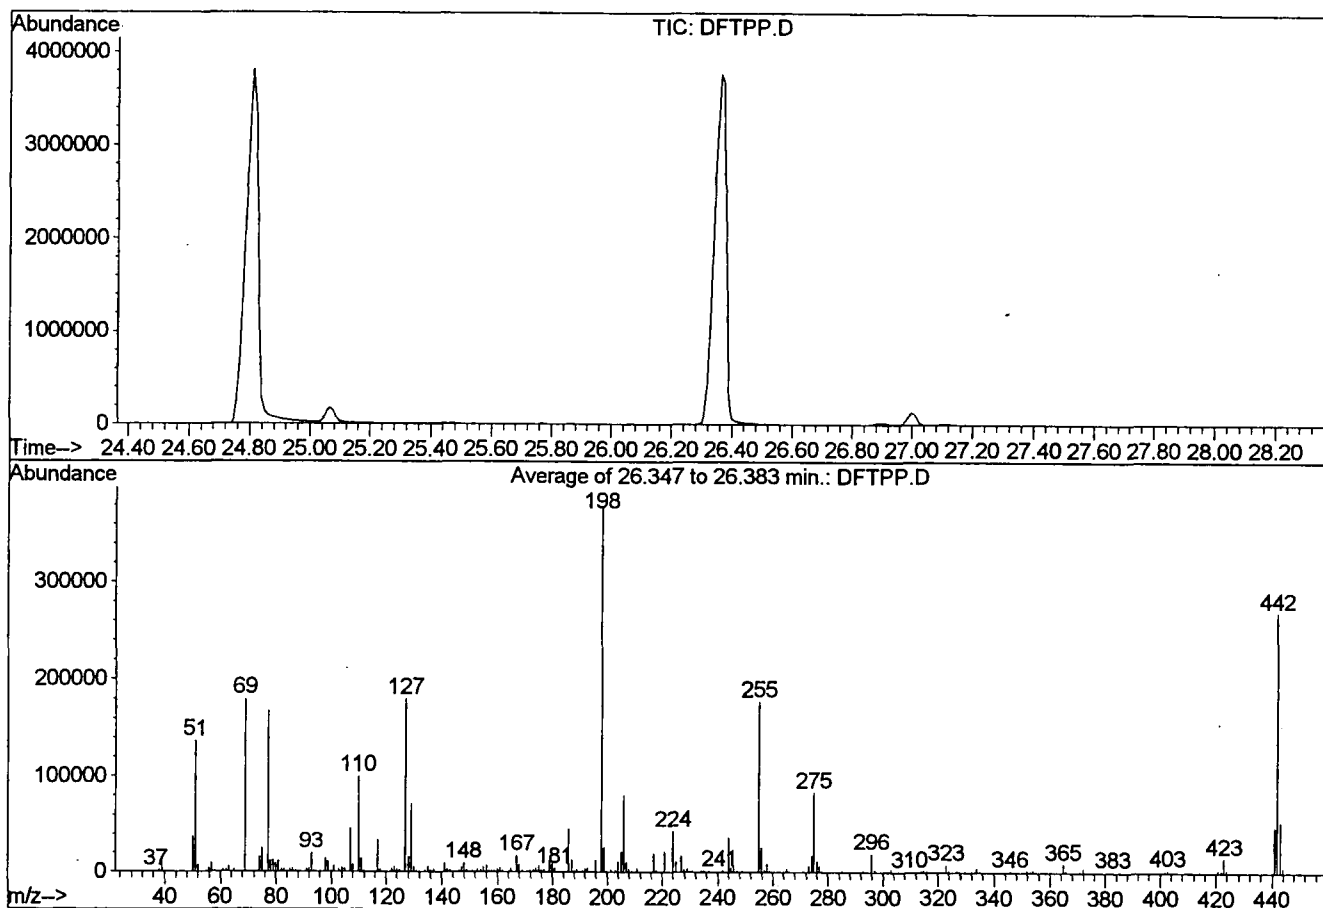

Spectrum Information: Average of 26.347 to 26.383 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	36.0	136315	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	47.3	179229	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	47.4	179574	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	378816	PASS
199	198	5	9	6.6	25015	PASS
275	198	10	30	22.0	83405	PASS
365	198	1	100	2.2	8463	PASS
441	443	0.01	100	89.1	46782	PASS
442	198	40	110	71.0	269005	PASS
443	442	17	23	19.5	52499	PASS

DFTPP.D NP091101.M

Tue Oct 02 11:57:32 2001

DFTPP

Data File : C:\HPCHEM\1\DATA\SEP2601\DFTPP.D

Acq On : 26 Sep 2001 10:28 am

Sample :

Misc :

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\NP072501.M (RTE Integrator)


Title : 208 625/TCLP calibration table 7/25/01 C1 IS 5

Vial: 1

Operator: GALOS

Inst : GC/MS Ins

Multiplr: 1.00

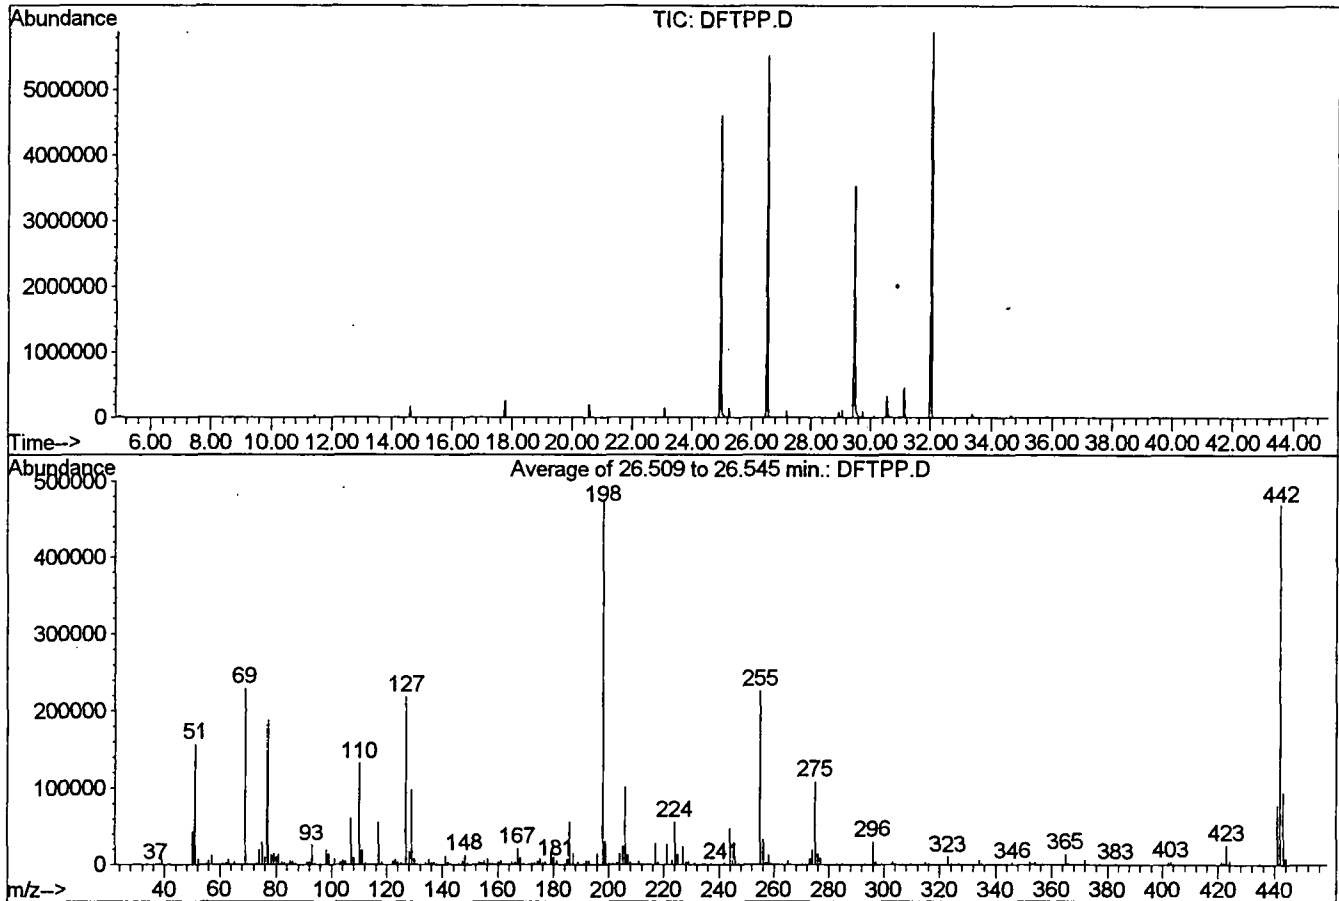

Spectrum Information: Average of 26.509 to 26.545 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	33.0	157200	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	48.2	229744	PASS
70	69	0.00	2	0.4	921	PASS
127	198	40	60	45.9	218816	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	476544	PASS
199	198	5	9	6.6	31468	PASS
275	198	10	30	22.8	108565	PASS
365	198	1	99	2.9	13753	PASS
441	443	1	99	82.4	77637	PASS
442	198	40	110	98.7	470323	PASS
443	442	17	23	20.0	94200	PASS

DFTPP.D NP072501.M

Wed Sep 26 11:21:22 2001