

Tentatively Identified Compound (LSC) summary

For ID: 209 GALOS Date Acquired: 2 Oct 2001 3:06 pm
 File: C:\HPCHEM\1\DATA\OCT0201\LB.D
 Date: 9/20
 Method: C:\HPCHEM\1\METHODS\NP091101.M (RTE Integrator)
 Title: 209 625/TCLP calibration table 7/16/01/
 Library Searched: C:\DATABASE\NBS75K.L

My Sheet
Lab Blank

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
Hexanone	6.38	0.6	ug/l	76825	ISTD01	11.78	2566400	20.0
Hexanone	6.49	0.8	ug/l	107024	ISTD01	11.78	2566400	20.0
Hexanol	6.62	0.4	ug/l	53199	ISTD01	11.78	2566400	20.0
Hexanol	6.74	0.7	ug/l	88381	ISTD01	11.78	2566400	20.0
1,4-Dichlorobenzene	11.64	0.5	ug/l	69043	ISTD01	11.78	2566400	20.0
Nonpentanecarboxyl	29.54	1.7	ug/l	260921	ISTD05	33.16	3048400	20.0
triacontane	30.73	0.6	ug/l	84270	ISTD05	33.16	3048400	20.0
adecanoic acid, 2	31.67	1.3	ug/l	204617	ISTD05	33.16	3048400	20.0
tricosane	31.77	1.2	ug/l	179169	ISTD05	33.16	3048400	20.0
eicosane	32.76	1.2	ug/l	183463	ISTD05	33.16	3048400	20.0
tacosane	33.72	1.5	ug/l	221588	ISTD05	33.16	3048400	20.0
racosane	34.63	1.1	ug/l	168992	ISTD05	33.16	3048400	20.0
racosane	35.53	1.1	ug/l	147163	ISTD06	37.28	2788270	20.0
triacontane	36.39	0.7	ug/l	93256	ISTD06	37.28	2788270	20.0

3.D NP091101.M Wed Oct 03 10:10:14 2001

29.20 Benzidine

27.12 Di n butyl phthalate

30.73 ? 22914

33.41 22915

Is { 1,4 DCB 11.78
 Nap 15.40
 Ace nap 20.69
 Phenol 25.11
 Chrysene 33.16
 Pyrene 37.23

QC Reviewed by:
[Signature] 11/30/01

Method

508 / nyc

Date Extracted

9620101

Page

90

GP/MS unknown

[illegible]

Analyst mmt
revision: 10/15/99

Verified by _____

Supv. approved

DW
10/8/11

Sequence Name: C:\HPCHEM\1\SEQUENCE\oct0201.S

Comment: INST 209; 30Mx0.25umX0.50

Operator: 209 GALOS

Data Path: C:\HPCHEM\1\data\oct0201\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run

On A Barcode Mismatch

☒ Full Method☒ Inject Anyway☐ Reprocessing Only☐ Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
------	------	------	----------	--------	-------------

1	Sample	1	DFTPP	NP091101	
2	Sample	2	LB ✓	NP091101	9/20
3	Sample	3	22913 ✓	NP091101	gc/ms unknown
4	Sample	4	22914 ✓	NP091101	gc/ms unknown
5	Sample	5	22915 ✓	NP091101	gc/ms unknown
6	Sample	6	22916 ✓	NP091101	gc/ms unknown
7	Sample	7	22917 ✓	NP091101	gc/ms unknown
8	Sample	8	22918 ✓	NP091101	gc/ms unknown
9	Sample	9	22919 ✓	NP091101	gc/ms unknown
10	Sample	10	22974	NP091101	gc/ms unknown
11	Sample	11	22975 ✓	NP091101	gc/ms unknown
12	Sample	12	22775 ✓	NP091101	gc/ms unknown
13	Sample	13	22776 ✓	NP091101	gc/ms unknown
14	Sample	14	22777 ✓	NP091101	gc/ms unknown
15	Sample	15	22778 ✓	NP091101	gc/ms unknown
16	Sample	16	22779 ✓	NP091101	gc/ms unknown
17					

needs 15
needs 15
included in 10/4/06
sequence

DFTPP

Data File : C:\HPCHEM\1\DATA\OCT0201\DFTPP.D

Acq On : 2 Oct 2001 12:19 pm

Sample :

Misc :

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\NP091101.M (RTE Integrator)


Title : 209 625/TCLP calibration table 7/16/01

Vial: 1

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

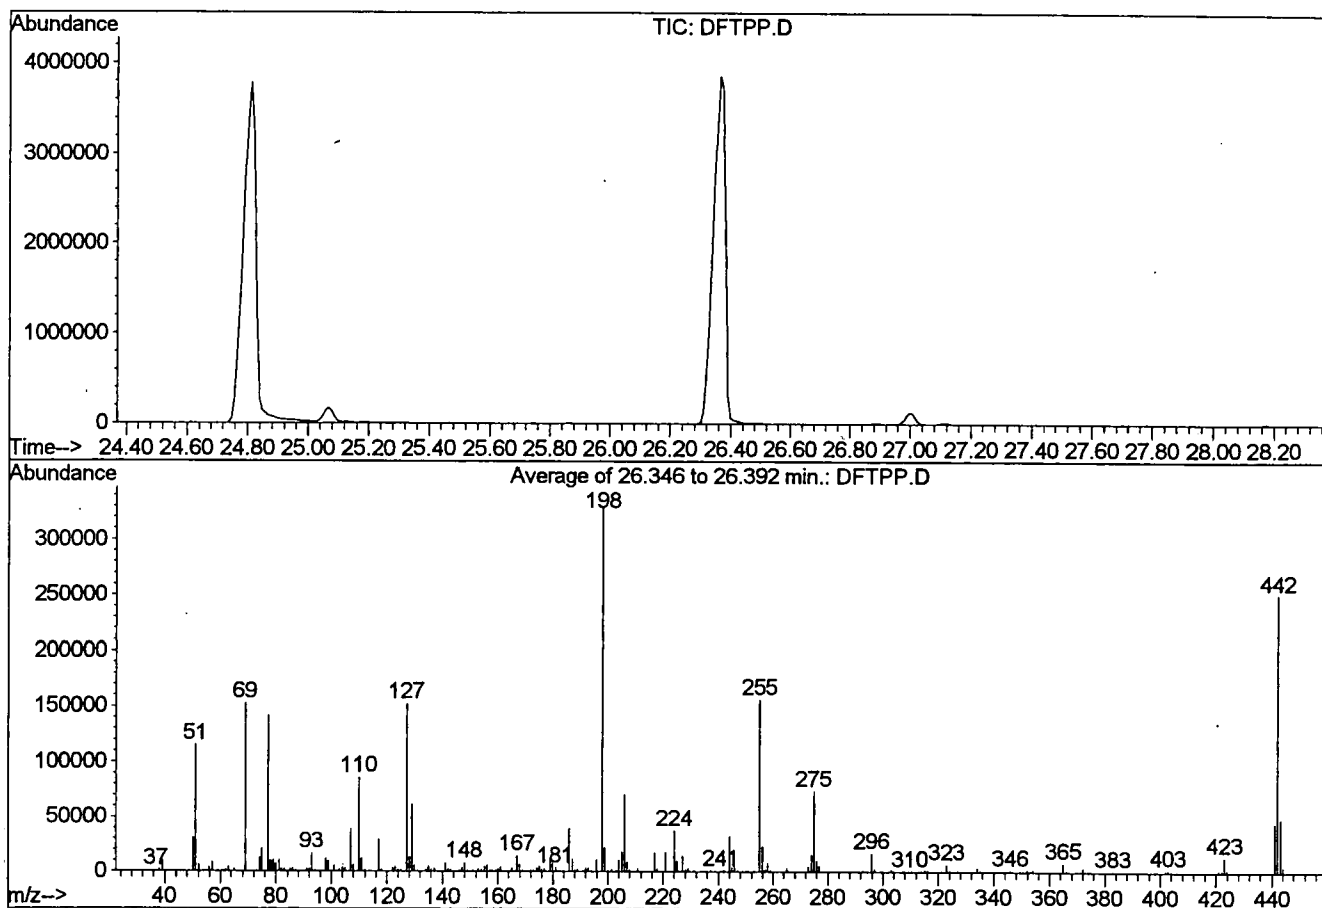

Spectrum Information: Average of 26.346 to 26.392 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	34.8	114849	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.2	152532	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	46.0	151967	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	330155	PASS
199	198	5	9	6.5	21563	PASS
275	198	10	30	22.4	73816	PASS
365	198	1	100	2.3	7549	PASS
441	443	0.01	100	91.4	44146	PASS
442	198	40	110	75.9	250727	PASS
443	442	17	23	19.3	48320	PASS