

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\OCT0201\22775.D

Vial: 12

Acq On : 3 Oct 2001 12:52 am

Operator: 209 GALOS

Sample : gc/ms unknown

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Oct 4 10:45 2001

Quant Results File: NP091101.RES

Quant Method : C:\HPCHEM\1\METHODS\NP091101.M (RTE Integrator)

Title : 209 625/TCLP calibration table 7/16/01

Last Update : Thu Sep 13 12:47:04 2001

Response via : Initial Calibration

DataAcq Meth : NP091101

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	11.79	152	466962	20.00	ug/l	-0.12
19) Naphthalene-d8	15.40	136	1837077	20.00	ug/l	-0.12
31) Acenaphthene-d10	20.68	164	871098	20.00	ug/l	-0.13
49) Phenanthrene-d10	25.11	188	1235856	20.00	ug/l	-0.12
59) Chrysene-d12	33.16	240	920144	20.00	ug/l	-0.12
68) Perylene-d12	37.27	264	697293	20.00	ug/l	-0.15

System Monitoring Compounds

4) 2-Fluorophenol	0.00	112	0	0.00	ug/l	
Spiked Amount	75.000		Recovery	=	0.00%	
5) Phenol-d5	0.00	99	0	0.00	ug/l	
Spiked Amount	75.000		Recovery	=	0.00%	
6) 2-Chlorophenol-d4	0.00	132	0	0.00	ug/l	
Spiked Amount	75.000		Recovery	=	0.00%	
7) 1,2-Dichlorobenzene-d4	12.31	152	4647	0.20	ug/l	-0.12
Spiked Amount	50.000		Recovery	=	0.40%	
20) Nitrobenzene-d5	0.00	82	0	0.00	ug/l	
Spiked Amount	50.000		Recovery	=	0.00%	
32) 2-Fluorobiphenyl	18.83	172	1727	0.03	ug/l	0.01
Spiked Amount	50.000		Recovery	=	0.06%	
33) 2,4,6-Tribromophenol	0.00	330	0	0.00	ug/l	
Spiked Amount	75.000		Recovery	=	0.00%	
62) Terphenyl-d14	0.00	244	0	0.00	ug/l	
Spiked Amount	50.000		Recovery	=	0.00%	

Target Compounds

Qvalue

2) Pyridine	0.00	79	0	N.D.	
3) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
8) Phenol	0.00	94	0	N.D.	
9) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
10) 2-Chlorophenol	0.00	128	0	N.D.	
11) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
12) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
13) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
14) 2-Methylphenol	0.00	108	0	N.D.	
15) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
16) 3&4-Methylphenol	0.00	108	0	N.D.	
17) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
18) Hexachloroethane	0.00	117	0	N.D.	
21) Nitrobenzene	0.00	77	0	N.D.	
22) Isophorone	0.00	82	0	N.D.	

(#)= qualifier out of range (m) = manual integration

22775.D NP091101.M Thu Oct 04 10:45:54 2001

Page 1

Quantitation Report (QT Reviewed)

Data File : C:\HPCHEM\1\DATA\OCT0201\22775.D
 Acq On : 3 Oct 2001 12:52 am
 Sample : gc/ms unknown
 Misc :
 MS Integration Params: RTEINT.P
 Quant Time: Oct 4 10:45 2001

Vial: 12
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: NP091101.RES

Quant Method : C:\HPCHEM\1\METHODS\NP091101.M (RTE Integrator)
 Title : 209 625/TCLP calibration table 7/16/01
 Last Update : Thu Sep 13 12:47:04 2001
 Response via : Initial Calibration
 DataAcq Meth : NP091101

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
23) 2-Nitrophenol	0.00	139	0	N.D.		
24) 2,4-Dimethylphenol	0.00	107	0	N.D.		
25) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.		
26) 2,4-Dichlorophenol	0.00	162	0	N.D.		
27) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.		
28) Naphthalene	0.00	128	0	N.D.		
29) Hexachlorobutadiene	0.00	225	0	N.D.		
30) 4-Chloro-3-methylphenol	0.00	107	0	N.D.		
34) Hexachlorocyclopentadiene	0.00	237	0	N.D.		
35) 2,4,6-Trichlorophenol	0.00	196	0	N.D.		
36) 2,4,5-Trichlorophenol	0.00	196	0	N.D.		
37) 2-Chloronaphthalene	0.00	162	0	N.D.		
38) Dimethylphthalate	0.00	163	0	N.D.		
39) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d	
40) Acenaphthylene	0.00	152	0	N.D.		
41) Acenaphthene	0.00	153	0	N.D.		
42) 2,4-Dinitrophenol	0.00	184	0	N.D.		
43) 4-Nitrophenol	0.00	65	0	N.D.		
44) 2,4-Dinitrotoluene	0.00	165	0	N.D.		
45) Diethylphthalate	0.00	149	0	N.D.		
46) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.		
47) Fluorene	0.00	166	0	N.D.		
48) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.		
50) 4,6-Dinitro-2-methylphenol	0.00	198	0	N.D.		
51) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
52) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
53) Hexachlorobenzene	0.00	284	0	N.D.		
54) Pentachlorophenol	0.00	266	0	N.D.		
55) Phenanthrene	25.11	178	218	N.D.		
56) Anthracene	25.11	178	218	N.D.		
57) Di-n-butylphthalate	27.11	149	1367	N.D.		
58) Fluoranthene	0.00	202	0	N.D.		
60) 3,3'-Dichlorobenzidine	0.00	252	0	N.D.		
61) Benzidine	0.00	184	0	N.D.		
63) Pyrene	0.00	202	0	N.D.		
64) Butylbenzylphthalate	0.00	149	0	N.D.		
65) Benzo(a)anthracene	33.15	228	2234	N.D.		
66) Bis(2-ethylhexyl)phthalate	33.41	149	2397	N.D.		
67) Chrysene	33.15	228	2234	N.D.		
69) Di-n-Octylphthalate	0.00	149	0	N.D.		
70) Benzo(b)fluoranthene	0.00	252	0	N.D.		

(#) = qualifier out of range (m) = manual integration

22775.D NP091101.M Thu Oct 04 10:46:00 2001

Page 2

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\OCT0201\22775.D

Vial: 12

Acq On : 3 Oct 2001 12:52 am

Operator: 209 GALOS

Sample : gc/ms unknown

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Oct 4 10:45 2001

Quant Results File: NP091101.RES

Quant Method : C:\HPCHEM\1\METHODS\NP091101.M (RTE Integrator)

Title : 209 625/TCLP calibration table 7/16/01

Last Update : Thu Sep 13 12:47:04 2001

Response via : Initial Calibration

DataAcq Meth : NP091101

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
71) Benzo(k)fluoranthene	0.00	252	0	N.D.		
72) Benzo(a)pyrene	37.27	252	2555	N.D.		
73) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
74) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
75) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

22775.D NP091101.M Thu Oct 04 10:46:01 2001

Page 3

Quantitation Report

Data File : C:\HPCHEM\1\DATA\OCT0201\22775.D

Acq On : 3 Oct 2001 12:52 am

Sample : gc/ms unknown

Misc :

MS Integration Params: RTEINT.P

Quant Time: Oct 4 10:45 2001

Vial: 12

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00


Quant Results File: NP091101.RES

Method : C:\HPCHEM\1\METHODS\NP091101.M (RTE Integrator)

Title : 209 625/TCLP calibration table 7/16/01

Last Update : Thu Sep 13 12:47:04 2001

Response via : Initial Calibration

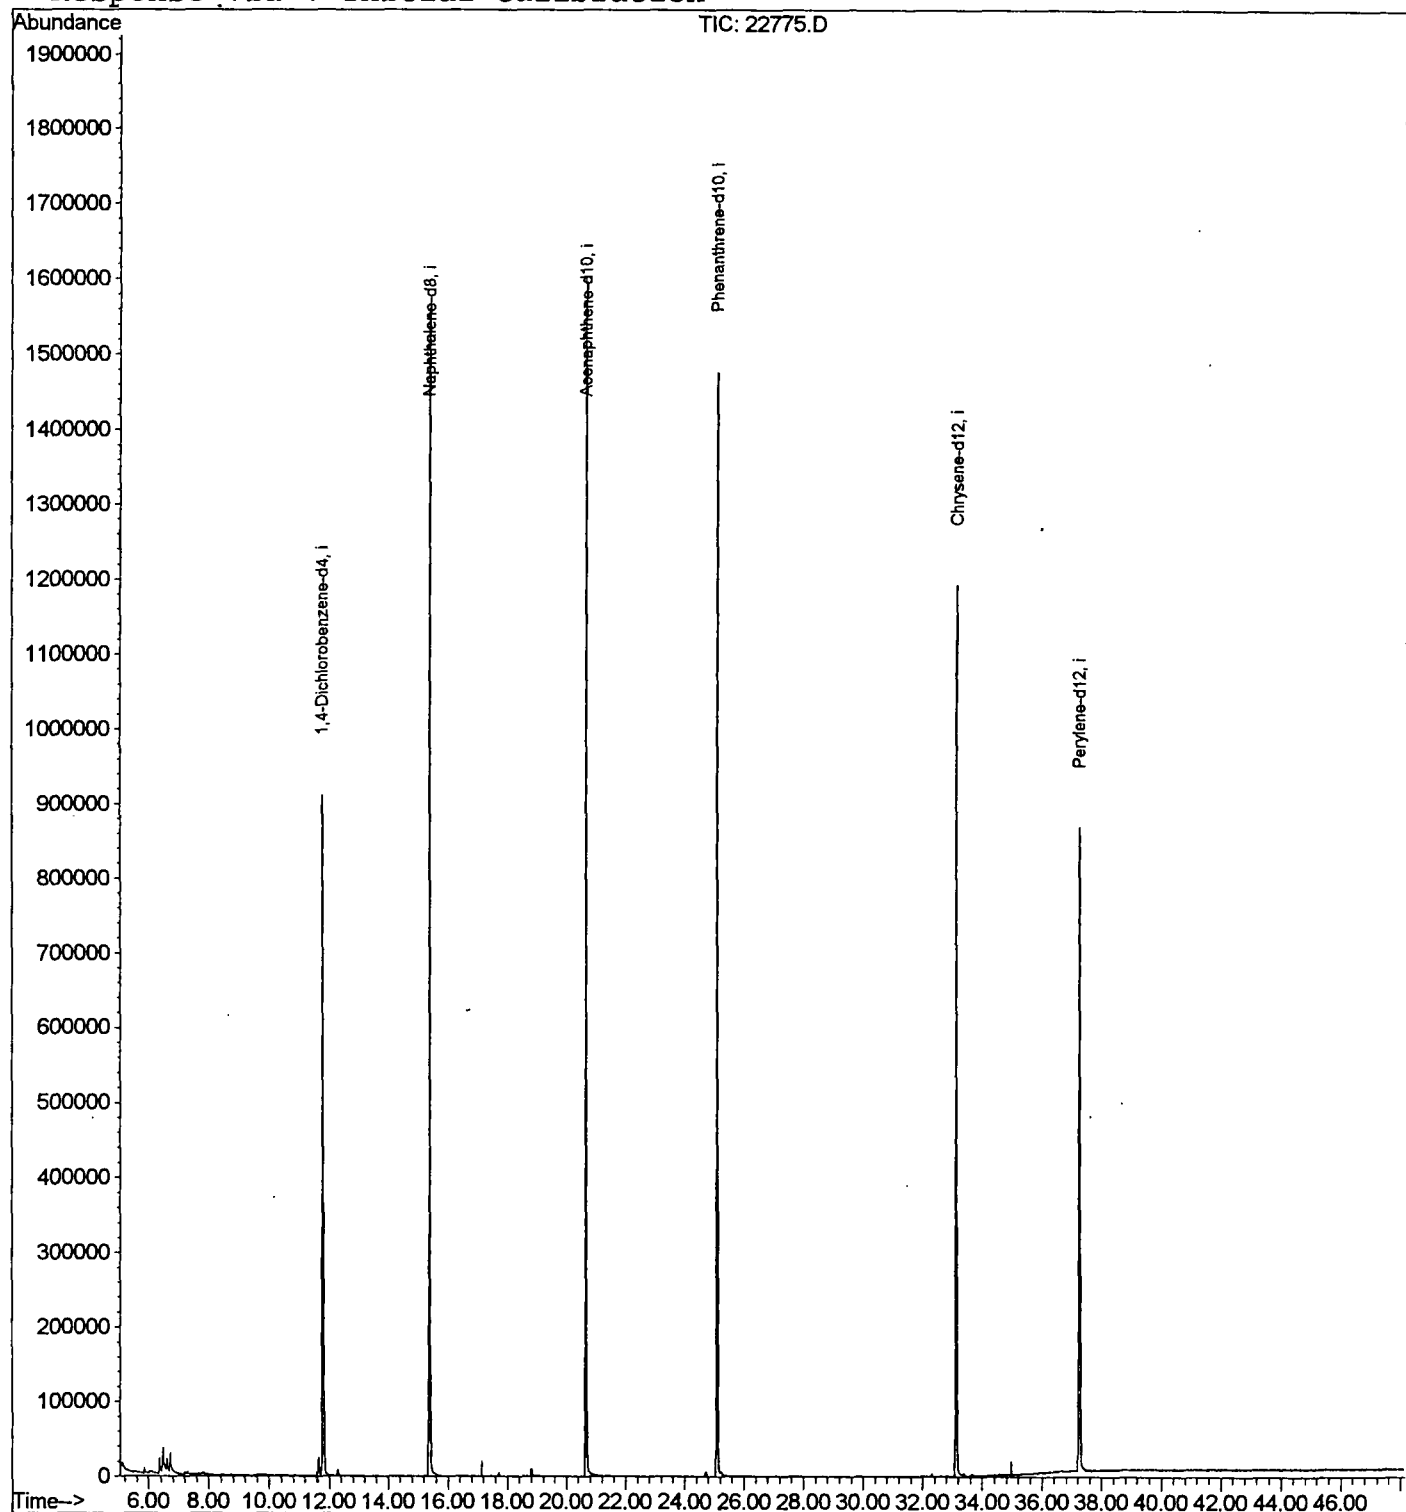

22775.D NP091101.M

Thu Oct 04 10:46:06 2001

Page 4

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\OCT0201\22775.D

Acq On : 3 Oct 2001 12:52 am

Sample : gc/ms unknown

Misc :

MS Integration Params: LSCINT.P

Vial: 12

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\NP091101.M (RTE Integrator)

Title : 209 625/TCLP calibration table 7/16/01

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	6.369	141	145	149	rBV	21019	42650	1.23%	0.236%
2	6.470	153	156	160	rBV	30357	63374	1.83%	0.351%
3	6.607	168	171	180	rVB	15941	37788	1.09%	0.209%
4	6.727	180	184	190	rBV	23531	49054	1.42%	0.272%
5	11.647	715	720	729	rVB	25117	64256	1.85%	0.356%
6	11.785	729	735	751	rBV	909676	2426333	70.00%	13.446%
7	15.402	1122	1129	1147	rBV	1562793	3340080	96.37%	18.510%
8	20.681	1698	1704	1725	rBV	1603159	3466045	100.00%	19.208%
9	25.115	2180	2187	2197	rBV	1475290	3167351	91.38%	17.553%
10	33.157	3055	3063	3081	rBV2	1190082	2856760	82.42%	15.831%
11	37.270	3502	3511	3524	rBV2	859747	2531117	73.03%	14.027%


Sum of corrected areas: 18044808

22775.D NP091101.M

Thu Oct 04 10:46:47 2001

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\OCT0201\22775.D
 Operator : 209 GALOS
 Acquired : 3 Oct 2001 12:52 am using AcqMethod NP091101
 Instrument : GC/MS 209
 Sample Name: gc/ms unknown
 Misc Info :
 Vial Number: 12
 Quant File :NP091101.RES (RTE Integrator)

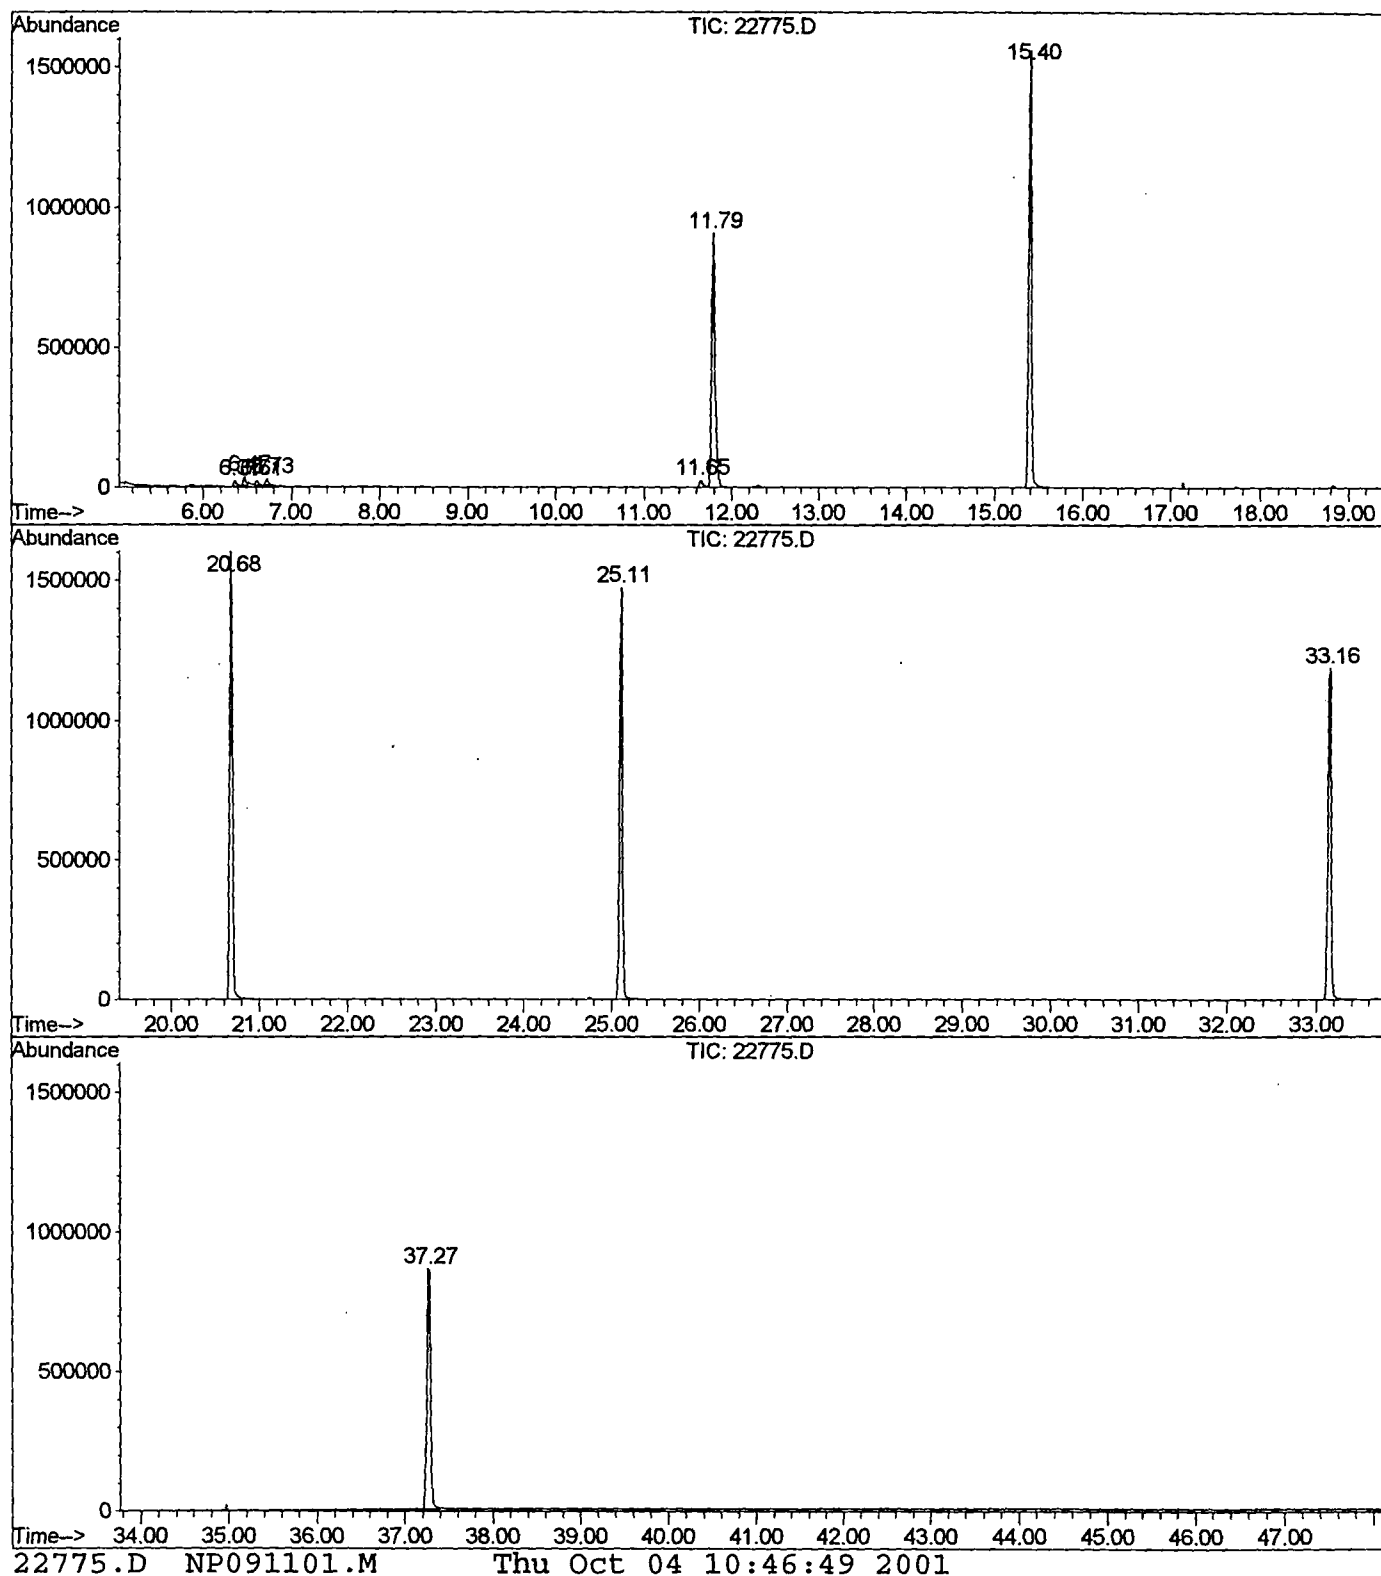

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\OCT0201\22775.D
Acq On : 3 Oct 2001 12:52 am
Sample : gc/ms unknown
Misc :
MS Integration Params: LSCINT.P


Vial: 12
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\NP091101.M (RTE Integrator)
Title : 209 625/TCLP calibration table 7/16/01
Library : C:\DATABASE\NBS75K.L

Peak Number 1 2-Hexanone Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.47	0.52 ug/l	63374	1,4-Dichlorobenzene-d4	11.79

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Hexanone	100	C6H12O	000591-78-6	86
2		Methyl Isobutyl Ketone	100	C6H12O	000108-10-1	58
3		Propanal	58	C3H6O	000123-38-6	43
4		2-Hexanone, 4-hydroxy-3-propyl-	158	C9H18O2	062338-17-4	40

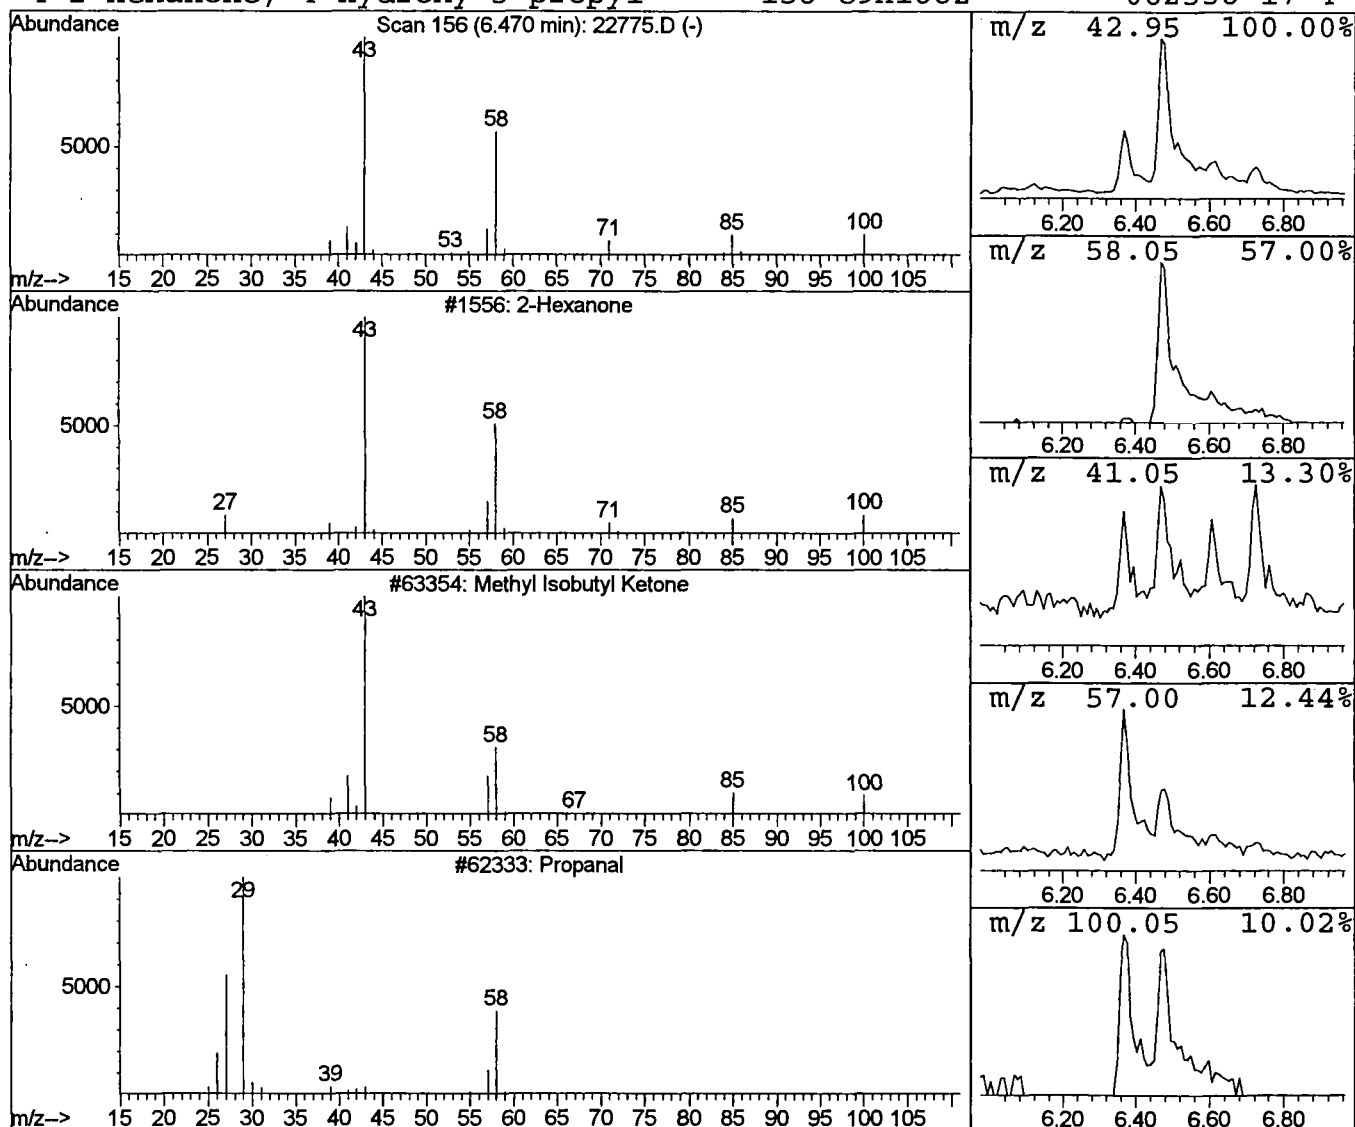

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\OCT0201\22775.D
 Acq On : 3 Oct 2001 12:52 am
 Sample : gc/ms unknown
 Misc :
 MS Integration Params: LSCINT.P


Vial: 12
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\NP091101.M (RTE Integrator)
 Title : 209 625/TCLP calibration table 7/16/01
 Library : C:\DATABASE\NBS75K.L

 Peak Number 2 2-Pentanol, 4-methyl- Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.73	0.40 ug/l	49054	1,4-Dichlorobenzene-d4	11.79

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanol, 4-methyl-	102	C6H14O	000108-11-2	83
2			2-Hexanol	102	C6H14O	000626-93-7	83
3			2-Hexanol, 3-methyl-	116	C7H16O	002313-65-7	40
4			2-Heptanol, 3-methyl-	130	C8H18O	031367-46-1	39

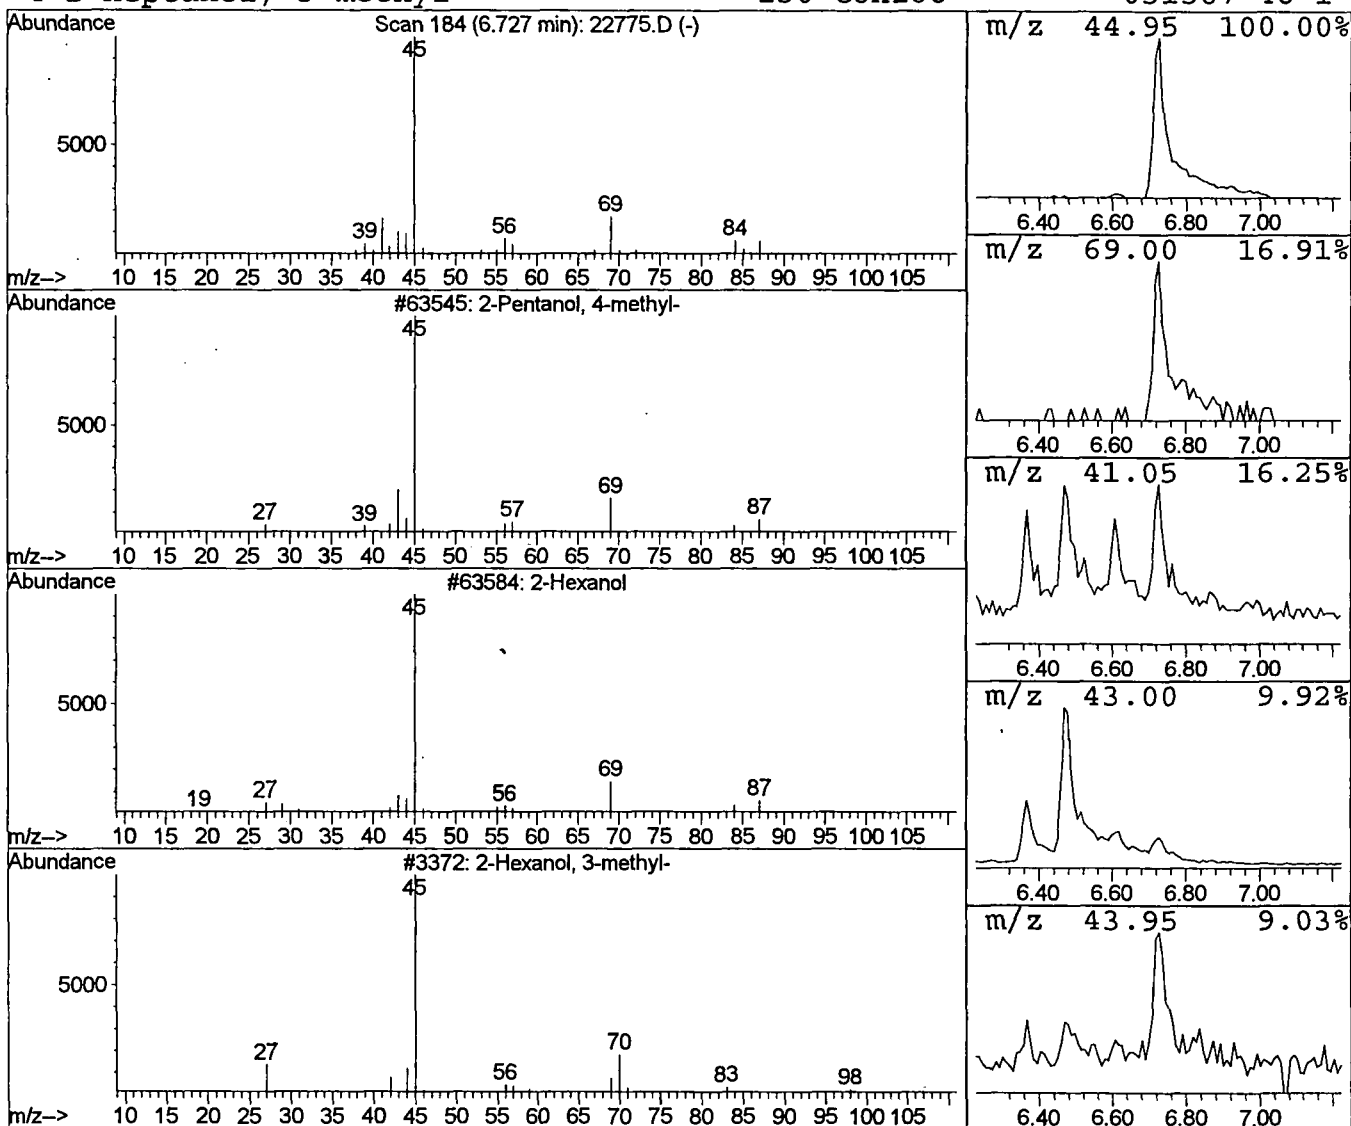

Library Search Compound Report


Data File : C:\HPCHEM\1\DATA\OCT0201\22775.D
Acq On : 3 Oct 2001 12:52 am
Sample : gc/ms unknown
Misc :
MS Integration Params: LSCINT.P

Vial: 12
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\NP091101.M (RTE Integrator)
Title : 209 625/TCLP calibration table 7/16/01
Library : C:\DATABASE\NBS75K.L

Peak Number 3 1,4-Dichlorobenzene-d4 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
11.65	0.53 ug/l	64256	1,4-Dichlorobenzene-d4	11.79	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	1,4-Dichlorobenzene-d4	150	C6Cl2D4	003855-82-1	50
2	Benzene-1,2,3,4-d4-, 5,6-dichloro-	150	C6Cl2D4	002199-69-1	45
3	2-Adamantanone	150	C10H14O	000700-58-3	25
4	Benzo[b]thiophene-4-ol	150	C8H6OS	003610-02-4	9

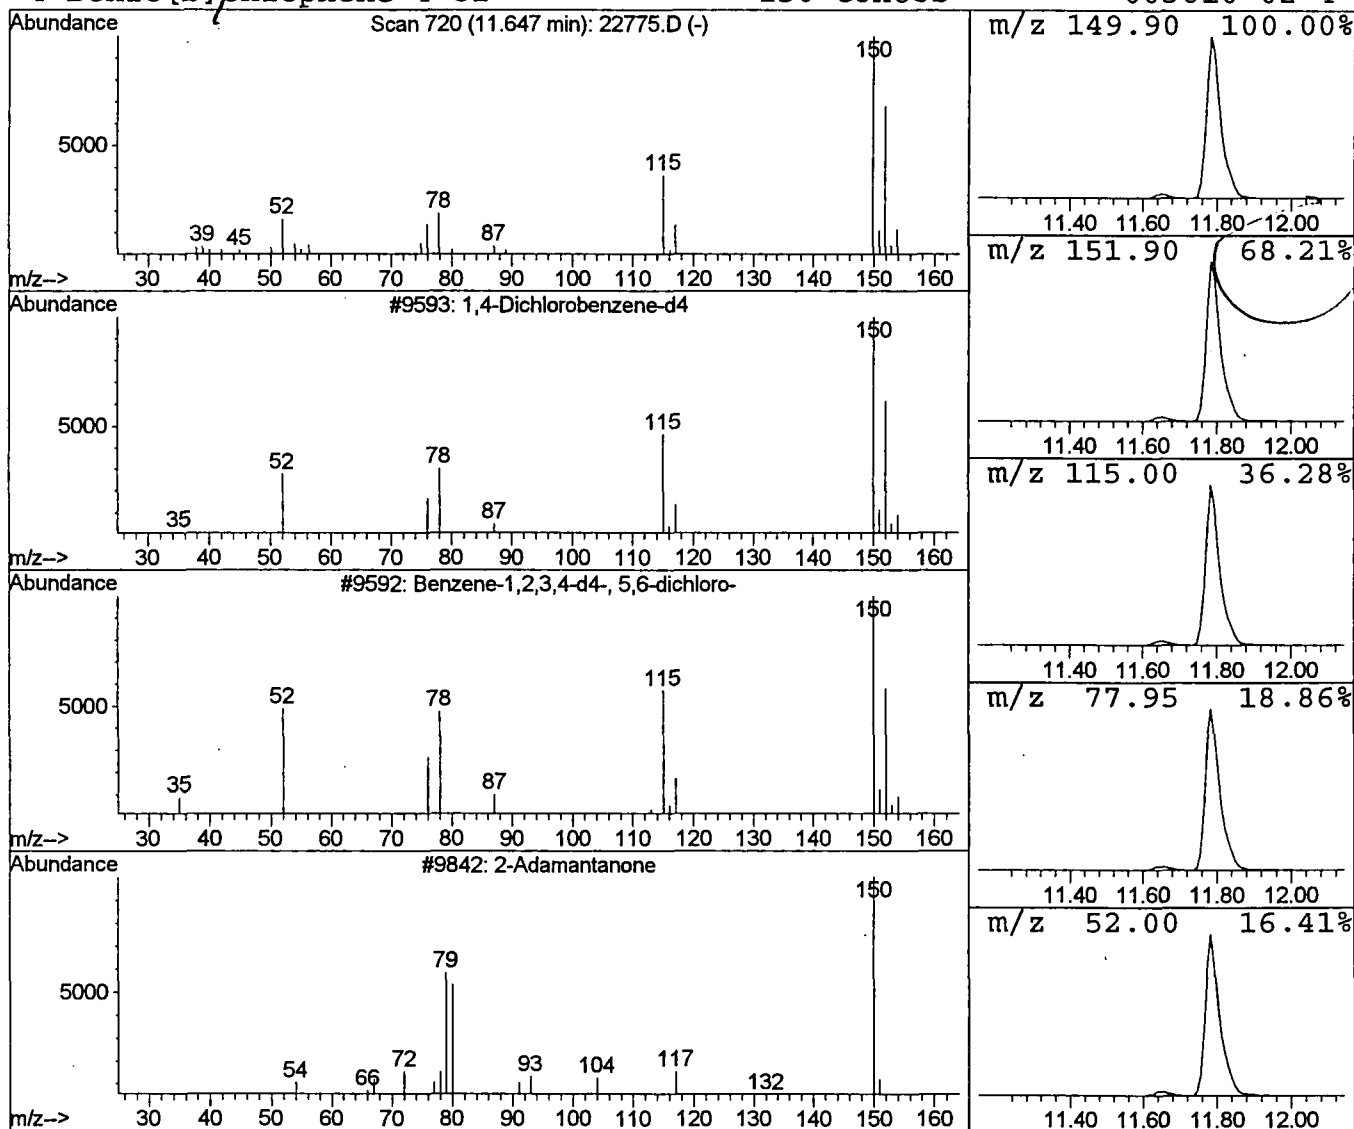

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 3 Oct 2001 12:52 am
 Data File: C:\HPCHEM\1\DATA\OCT0201\22775.D
 Name: gc/ms unknown
 Misc:
 Method: C:\HPCHEM\1\METHODS\NP091101.M (RTE Integrator)
 Title: 209 625/TCLP calibration table 7/16/01
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Hexanone	6.47	0.5	ug/l	63374	ISTD01	11.79	2426330	20.0
2-Pentanol, 4-methyl	6.73	0.4	ug/l	49054	ISTD01	11.79	2426330	20.0
1,4-Dichlorobenzene-	11.65	0.5	ug/l	64256	ISTD01	11.79	2426330	20.0

22775.D NP091101.M Thu Oct 04 10:46:58 2001

Comments for Sample AD22775 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 10-08-2001 Time: 12:17:40

A scan of the extract prepared for the 508 analysis, from 35 - 550 amu using a mass spectrometer, does not reveal the presence of any non-target compounds.